

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046979.D
 Acq On : 04 Aug 2024 00:50
 Operator : MA/JU
 Sample : P3276-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM046979.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.993	14	18	21	rBV3	25493	32936	1.14%	0.106%
2	3.022	21	23	30	rVB	23924	28943	1.00%	0.093%
3	3.281	64	67	68	rBV2	4102	4287	0.15%	0.014%
4	3.299	68	70	74	rVB2	5914	7331	0.25%	0.024%
5	3.410	86	89	103	rBV	257190	401241	13.92%	1.288%
6	3.710	137	140	148	rVB	12736	18040	0.63%	0.058%
7	4.081	199	203	206	rBV6	2756	3642	0.13%	0.012%
8	4.463	265	268	270	rBV4	3484	4002	0.14%	0.013%
9	4.593	288	290	294	rVB5	3619	3926	0.14%	0.013%
10	4.840	329	332	335	rBV5	2730	4079	0.14%	0.013%
11	5.140	381	383	385	rBV2	2883	2943	0.10%	0.009%
12	5.540	449	451	456	rBV6	4708	8252	0.29%	0.026%
13	6.492	610	613	615	rVB4	3232	2946	0.10%	0.009%
14	6.604	626	632	642	rVB	360753	558279	19.37%	1.791%
15	6.757	650	658	667	rBV	315269	484604	16.81%	1.555%
16	6.940	682	689	701	rBV	392386	607625	21.08%	1.950%
17	7.222	734	737	742	rBV5	3891	7125	0.25%	0.023%
18	7.398	760	767	777	rBV	795980	1223412	42.44%	3.926%
19	7.481	777	781	786	rVV5	4666	9820	0.34%	0.032%
20	8.116	882	889	897	rBV	441442	708828	24.59%	2.275%
21	8.239	908	910	913	rVB4	3085	3054	0.11%	0.010%
22	8.539	955	961	972	rVB	361147	588734	20.43%	1.889%
23	8.722	987	992	994	rVB6	3078	3335	0.12%	0.011%
24	8.992	1033	1038	1045	rVB8	4902	8667	0.30%	0.028%
25	9.128	1054	1061	1068	rBV3	17895	32581	1.13%	0.105%
26	9.257	1076	1083	1091	rBV	296626	481218	16.70%	1.544%
27	9.675	1151	1154	1156	rBV4	2901	3702	0.13%	0.012%
28	9.792	1166	1174	1184	rBV	457235	751432	26.07%	2.411%
29	10.157	1227	1236	1245	rBV	1024257	1665865	57.79%	5.346%
30	10.304	1254	1261	1270	rBV	440635	739393	25.65%	2.373%
31	10.745	1329	1336	1338	rBV6	3255	5923	0.21%	0.019%
32	10.916	1359	1365	1378	rBV2	31038	69236	2.40%	0.222%
33	11.751	1505	1507	1515	rVB6	8986	14549	0.50%	0.047%
34	12.551	1639	1643	1645	rVB4	2426	3004	0.10%	0.010%
35	12.657	1658	1661	1665	rBV5	2598	3101	0.11%	0.010%
36	12.857	1692	1695	1699	rBV6	3065	4741	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046979.D
 Acq On : 04 Aug 2024 00:50
 Operator : MA/JU
 Sample : P3276-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

37	12.898	1699	1702	1706	rVB4	6199	8751	0.30%	0.028%
38	12.939	1706	1709	1712	rBV4	2579	4045	0.14%	0.013%
39	13.480	1795	1801	1811	rBV	842848	1161079	40.28%	3.726%
40	13.745	1839	1846	1857	rBV2	928038	1399084	48.54%	4.490%
41	13.992	1886	1888	1892	rVB4	3831	4339	0.15%	0.014%
42	14.057	1892	1899	1907	rBV	1533753	2221719	77.08%	7.129%
43	14.298	1933	1940	1952	rBV2	234869	445551	15.46%	1.430%
44	14.504	1973	1975	1978	rBV4	3602	4093	0.14%	0.013%
45	14.898	2036	2042	2047	rBV6	6759	9915	0.34%	0.032%
46	14.951	2047	2051	2054	rBV5	5099	6034	0.21%	0.019%
47	15.063	2063	2070	2078	rBV	1196517	1729177	59.99%	5.549%
48	15.198	2087	2093	2101	rBV	238624	339086	11.76%	1.088%
49	15.257	2101	2103	2106	rVB4	5613	6277	0.22%	0.020%
50	15.304	2108	2111	2115	rVB6	4825	5826	0.20%	0.019%
51	15.462	2135	2138	2140	rVB4	3485	3643	0.13%	0.012%
52	15.515	2146	2147	2152	rVB5	3116	3799	0.13%	0.012%
53	15.762	2185	2189	2192	rBV6	2935	3529	0.12%	0.011%
54	15.821	2195	2199	2203	rBV6	7621	14300	0.50%	0.046%
55	15.980	2221	2226	2228	rBV6	3740	6162	0.21%	0.020%
56	16.033	2230	2235	2239	rVV8	1524	3628	0.13%	0.012%
57	16.168	2254	2258	2259	rBV4	2476	2978	0.10%	0.010%
58	16.274	2273	2276	2280	rVB6	3724	6750	0.23%	0.022%
59	16.404	2295	2298	2301	rBV5	4814	5823	0.20%	0.019%
60	16.568	2323	2326	2329	rBV5	3328	4698	0.16%	0.015%
61	16.615	2329	2334	2338	rBV6	5762	12638	0.44%	0.041%
62	16.768	2357	2360	2361	rBV3	3307	2912	0.10%	0.009%
63	16.815	2362	2368	2374	rVV	1974173	2682068	93.05%	8.607%
64	16.915	2378	2385	2399	rVV	1347672	1918541	66.56%	6.156%
65	17.033	2403	2405	2410	rVB5	11139	14246	0.49%	0.046%
66	17.139	2417	2423	2425	rBV6	6720	10158	0.35%	0.033%
67	17.198	2430	2433	2436	rBV4	3439	5857	0.20%	0.019%
68	17.527	2483	2489	2492	rVB7	6215	11524	0.40%	0.037%
69	17.751	2522	2527	2537	rBV2	78181	138621	4.81%	0.445%
70	18.039	2574	2576	2578	rBV3	4141	4208	0.15%	0.014%
71	18.786	2700	2703	2708	rVB5	19517	24079	0.84%	0.077%
72	18.862	2712	2716	2720	rBV3	19344	29447	1.02%	0.094%
73	18.909	2720	2724	2726	rBV5	12576	20327	0.71%	0.065%
74	19.056	2745	2749	2754	rBV6	29011	47967	1.66%	0.154%
75	19.227	2772	2778	2787	rVB	1658574	2179062	75.60%	6.992%
76	19.321	2791	2794	2800	rVB6	28107	34022	1.18%	0.109%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046979.D
Acq On : 04 Aug 2024 00:50
Operator : MA/JU
Sample : P3276-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Title : SVOA CALIBRATION

77	20.792	3040	3044	3050	rBV3	133949	206239	7.16%	0.662%
78	21.050	3082	3088	3093	rBV	2119292	2882379	100.00%	9.249%
79	23.574	3511	3517	3529	rVB	1034636	2172125	75.36%	6.970%
80	23.762	3542	3549	3556	rBV	1341254	2865607	99.42%	9.196%




Sum of corrected areas: 31163109

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046979.D
Acq On : 04 Aug 2024 00:50
Operator : MA/JU
Sample : P3276-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

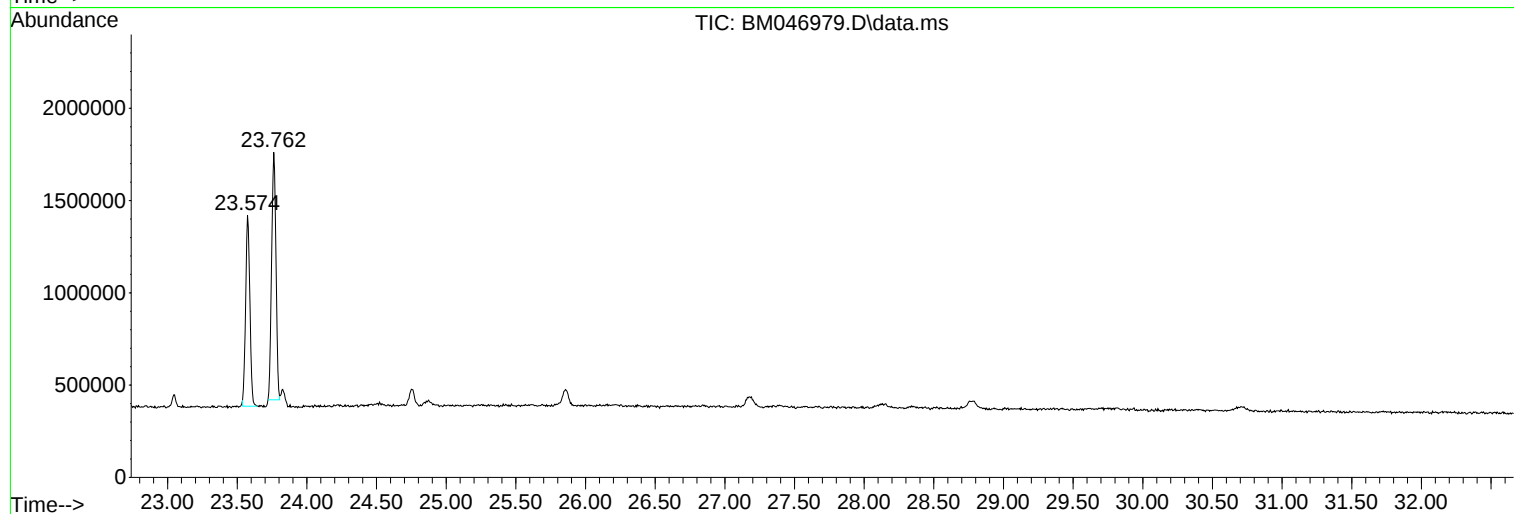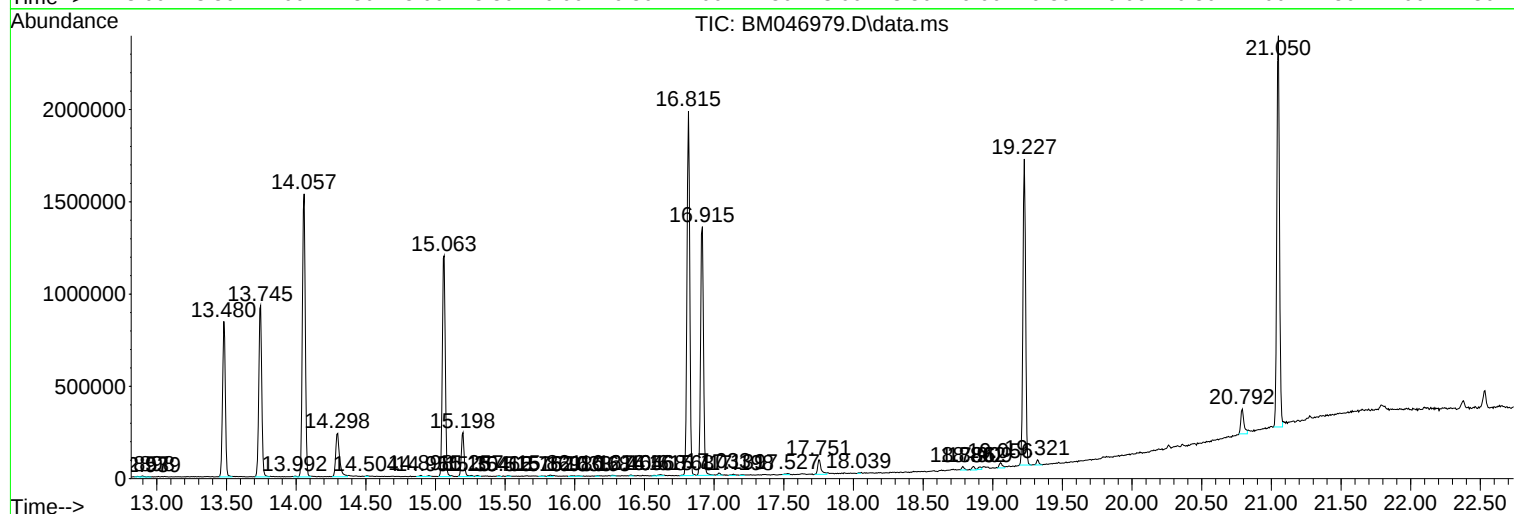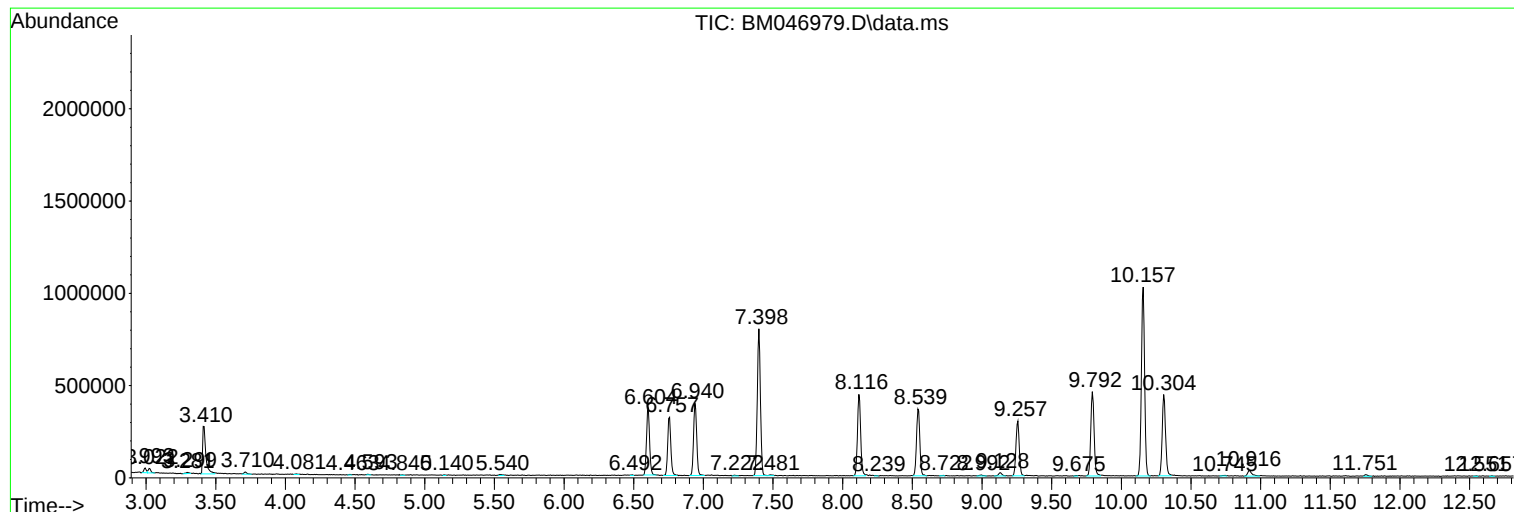

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046979.D
Acq On : 04 Aug 2024 00:50
Operator : MA/JU
Sample : P3276-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046979.D
Acq On : 04 Aug 2024 00:50
Operator : MA/JU
Sample : P3276-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc