

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046981.D
 Acq On : 04 Aug 2024 02:10
 Operator : MA/JU
 Sample : P3276-22
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM046981.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	19	23	28	rBV	37218	42298	1.39%	0.114%
2	3.210	53	55	58	rBV4	3179	3865	0.13%	0.010%
3	3.281	65	67	75	rBV	35420	51333	1.69%	0.138%
4	3.410	85	89	101	rBV	439239	609130	20.08%	1.637%
5	3.710	137	140	147	rVB4	11246	16608	0.55%	0.045%
6	3.928	175	177	180	rBV4	2201	3167	0.10%	0.009%
7	4.151	213	215	220	rVB6	2552	3194	0.11%	0.009%
8	4.593	286	290	295	rVB6	5067	9853	0.32%	0.026%
9	5.540	448	451	457	rVB3	7245	10312	0.34%	0.028%
10	5.693	475	477	482	rVB7	2371	3141	0.10%	0.008%
11	5.834	499	501	504	rBV4	2961	3993	0.13%	0.011%
12	6.110	544	548	552	rBV7	2854	3857	0.13%	0.010%
13	6.251	570	572	574	rBV2	3886	3304	0.11%	0.009%
14	6.457	602	607	608	rBV5	4002	4466	0.15%	0.012%
15	6.604	626	632	644	rBV	531271	834413	27.51%	2.243%
16	6.757	651	658	667	rVB	439244	682361	22.50%	1.834%
17	6.939	681	689	696	rBV	583594	870881	28.71%	2.341%
18	6.992	696	698	701	rVV4	4389	4050	0.13%	0.011%
19	7.051	703	708	710	rVB5	3929	6036	0.20%	0.016%
20	7.398	760	767	777	rBV	745643	1108475	36.55%	2.979%
21	7.487	778	782	783	rBV4	4584	5321	0.18%	0.014%
22	7.939	855	859	861	rVB5	2283	3133	0.10%	0.008%
23	8.116	883	889	898	rVV	670507	1039184	34.26%	2.793%
24	8.539	954	961	969	rBV	526865	849282	28.00%	2.283%
25	8.722	991	992	997	rVB5	4116	4149	0.14%	0.011%
26	8.992	1032	1038	1044	rVB8	6820	13104	0.43%	0.035%
27	9.128	1056	1061	1067	rBV3	21290	31082	1.02%	0.084%
28	9.257	1075	1083	1093	rBV	431921	714754	23.57%	1.921%
29	9.792	1166	1174	1184	rBV	678056	1095386	36.12%	2.944%
30	10.157	1228	1236	1243	rBV	925631	1530449	50.46%	4.113%
31	10.304	1252	1261	1274	rBV	632063	1061403	34.99%	2.853%
32	10.498	1293	1294	1296	rVB2	4755	3157	0.10%	0.008%
33	10.739	1328	1335	1339	rVB7	6542	13465	0.44%	0.036%
34	10.916	1359	1365	1375	rBV	50303	101703	3.35%	0.273%
35	10.998	1376	1379	1381	rVV4	4173	5466	0.18%	0.015%
36	11.016	1381	1382	1388	rVB6	2923	4247	0.14%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046981.D
 Acq On : 04 Aug 2024 02:10
 Operator : MA/JU
 Sample : P3276-22
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

37	11.210	1411	1415	1420	rVB7	2764	6360	0.21%	0.017%
38	11.610	1479	1483	1486	rBV5	2710	4114	0.14%	0.011%
39	11.692	1493	1497	1500	rBV4	2890	4077	0.13%	0.011%
40	11.757	1504	1508	1515	rBV3	12011	18811	0.62%	0.051%

41	12.186	1578	1581	1584	rBV4	2699	3425	0.11%	0.009%
42	12.604	1648	1652	1658	rVB8	3225	4502	0.15%	0.012%
43	12.663	1658	1662	1665	rBV5	4290	5916	0.20%	0.016%
44	12.857	1691	1695	1697	rBV4	3560	3907	0.13%	0.011%
45	12.898	1697	1702	1704	rVV4	6550	7695	0.25%	0.021%

46	13.033	1723	1725	1730	rVB6	2301	3265	0.11%	0.009%
47	13.268	1761	1765	1766	rBV4	3808	4646	0.15%	0.012%
48	13.480	1795	1801	1812	rBV	1159360	1592034	52.49%	4.279%
49	13.568	1814	1816	1820	rVB5	2735	3351	0.11%	0.009%
50	13.745	1839	1846	1855	rVV	1267684	1911310	63.02%	5.137%

51	13.810	1855	1857	1860	rVV4	3783	4278	0.14%	0.011%
52	13.933	1874	1878	1879	rVB4	3005	3501	0.12%	0.009%
53	13.951	1879	1881	1884	rBV4	2933	4098	0.14%	0.011%
54	13.992	1884	1888	1892	rBV5	6233	9415	0.31%	0.025%
55	14.057	1892	1899	1907	rBV	1351383	2026738	66.82%	5.447%

56	14.292	1933	1939	1955	rBV	432810	748025	24.66%	2.010%
57	14.504	1972	1975	1981	rVB7	4904	8318	0.27%	0.022%
58	14.698	2003	2008	2011	rVB7	2977	4336	0.14%	0.012%
59	14.892	2037	2041	2047	rVB8	8329	14751	0.49%	0.040%
60	14.951	2047	2051	2054	rVV6	7816	9421	0.31%	0.025%

61	15.057	2063	2069	2077	rBV	1610073	2315978	76.36%	6.225%
62	15.198	2087	2093	2100	rBV	396325	557377	18.38%	1.498%
63	15.298	2107	2110	2115	rVB4	10375	14655	0.48%	0.039%
64	15.362	2115	2121	2125	rBV7	4663	10465	0.35%	0.028%
65	15.462	2135	2138	2142	rVB6	5062	5449	0.18%	0.015%

66	15.510	2144	2146	2152	rVV7	3447	5785	0.19%	0.016%
67	15.651	2166	2170	2174	rVB7	3011	4257	0.14%	0.011%
68	15.721	2178	2182	2183	rBV3	4254	4551	0.15%	0.012%
69	15.821	2194	2199	2202	rBV4	9617	15950	0.53%	0.043%
70	15.974	2222	2225	2228	rVV5	2624	3765	0.12%	0.010%

71	16.192	2260	2262	2264	rVB3	4193	3425	0.11%	0.009%
72	16.227	2264	2268	2272	rBV6	4457	8257	0.27%	0.022%
73	16.268	2272	2275	2277	rBV4	7615	9775	0.32%	0.026%
74	16.351	2286	2289	2293	rVB5	3843	4593	0.15%	0.012%
75	16.404	2293	2298	2301	rBV7	6950	10438	0.34%	0.028%

76	16.498	2309	2314	2316	rBV6	2714	4787	0.16%	0.013%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046981.D
 Acq On : 04 Aug 2024 02:10
 Operator : MA/JU
 Sample : P3276-22
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

77	16.609	2328	2333	2339	rBV9	10041	16858	0.56%	0.045%
78	16.815	2362	2368	2374	rBV	1742842	2432319	80.19%	6.537%
79	16.915	2378	2385	2395	rBV	1831725	2534335	83.56%	6.811%
80	17.033	2401	2405	2410	rBV7	19270	26905	0.89%	0.072%
81	17.133	2418	2422	2425	rBV5	6147	7231	0.24%	0.019%
82	17.356	2457	2460	2465	rVB7	6584	10412	0.34%	0.028%
83	17.527	2486	2489	2492	rVB4	9923	11511	0.38%	0.031%
84	17.627	2503	2506	2511	rBV6	9751	14879	0.49%	0.040%
85	17.751	2523	2527	2536	rBV	157670	235633	7.77%	0.633%
86	18.298	2618	2620	2622	rBV3	4694	4116	0.14%	0.011%
87	18.786	2700	2703	2708	rVB3	22840	31334	1.03%	0.084%
88	18.856	2712	2715	2719	rBV	27191	32804	1.08%	0.088%
89	19.056	2745	2749	2754	rBV2	45968	72743	2.40%	0.196%
90	19.227	2772	2778	2784	rVB	2180117	2912724	96.03%	7.828%
91	20.792	3040	3044	3049	rBV2	236650	349716	11.53%	0.940%
92	21.050	3083	3088	3094	rBV	1926239	2588007	85.33%	6.956%
93	23.580	3511	3518	3529	rVB	1402292	3033045	100.00%	8.152%
94	23.762	3542	3549	3556	rBV	1250253	2756397	90.88%	7.408%




Sum of corrected areas: 37206792

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046981.D
Acq On : 04 Aug 2024 02:10
Operator : MA/JU
Sample : P3276-22
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

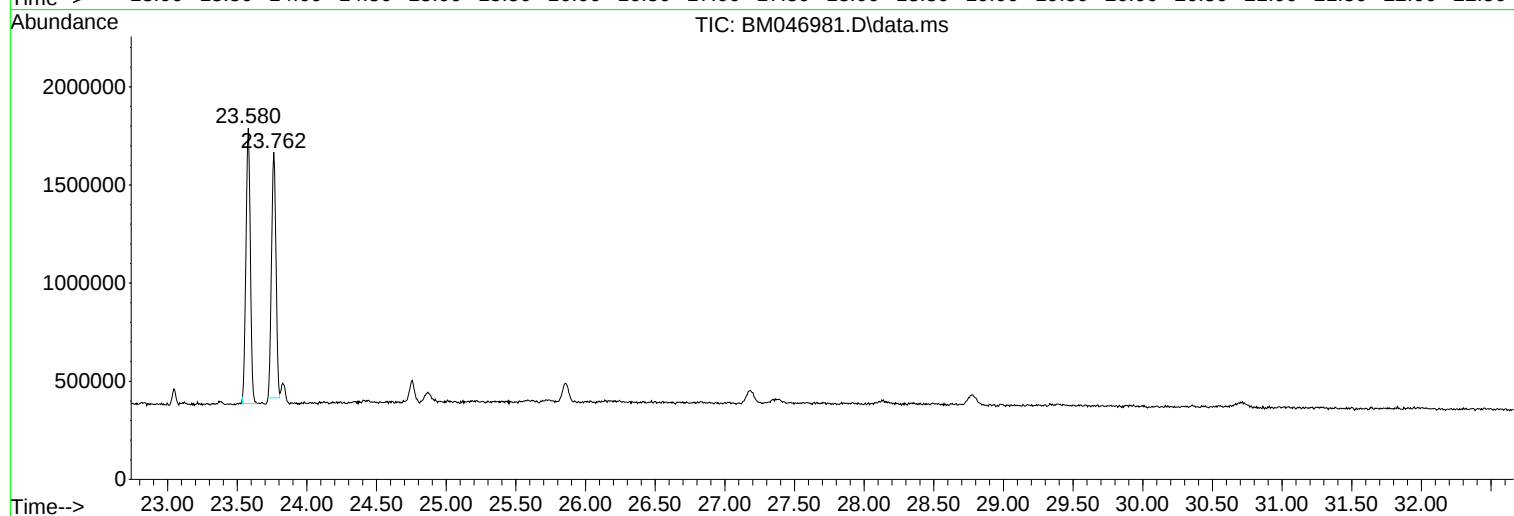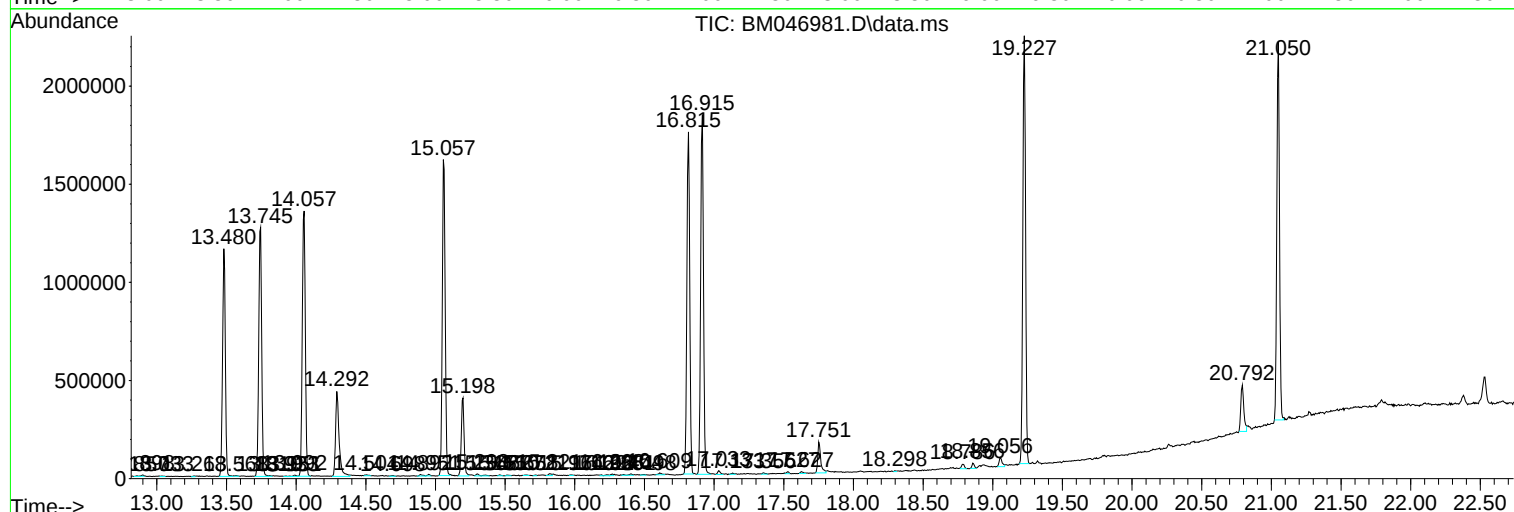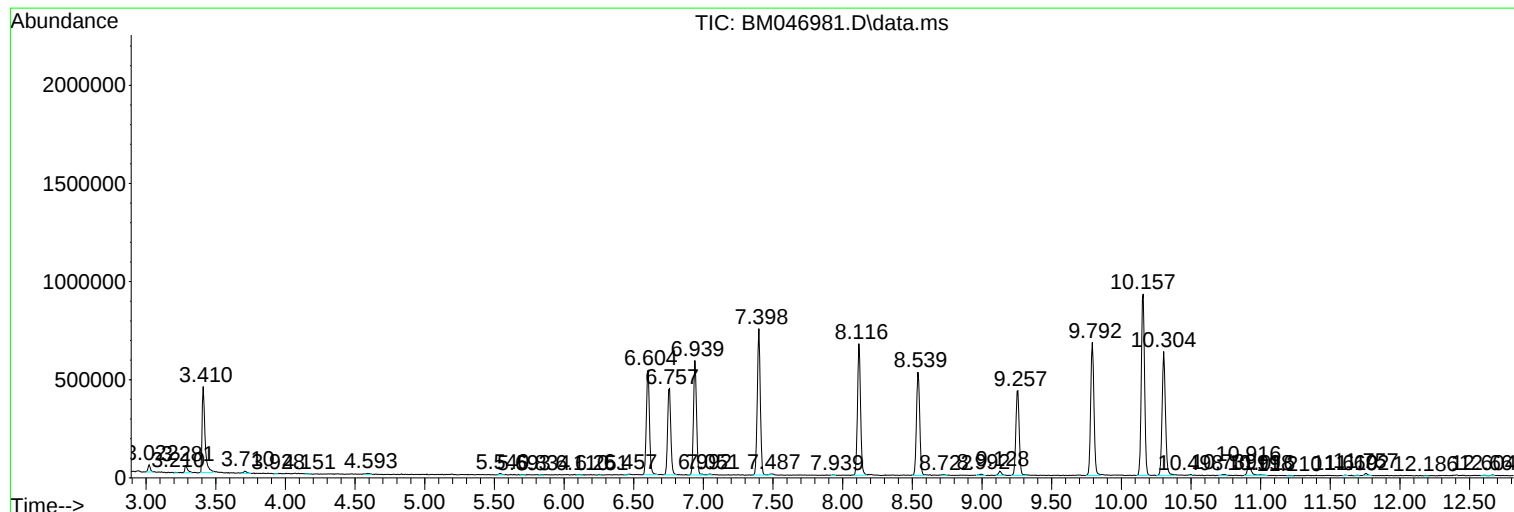

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046981.D
Acq On : 04 Aug 2024 02:10
Operator : MA/JU
Sample : P3276-22
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic20.791 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.791	2.70 ng/ul	349716	Chrysene-d12	21.050

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotridecane	182	C13H26	000295-02-3	95
2			1-Heneicosyl formate	340	C22H44O2	077899-03-7	95
3			Pentacos-1-ene	350	C25H50	016980-85-1	94
4			5-Octadecene, (E)-	252	C18H36	007206-21-5	93
5			Cyclopentadecane	210	C15H30	000295-48-7	93

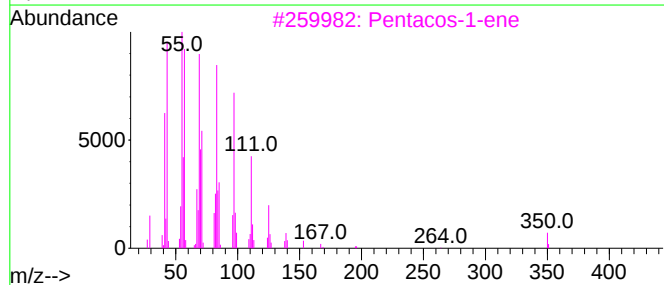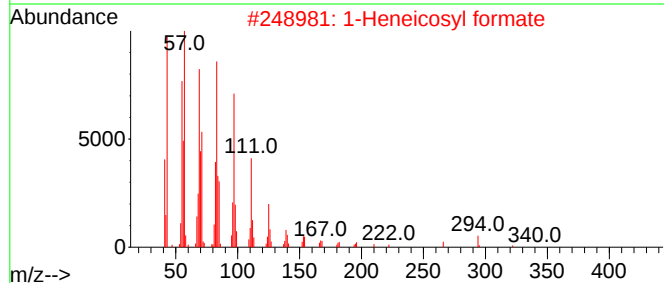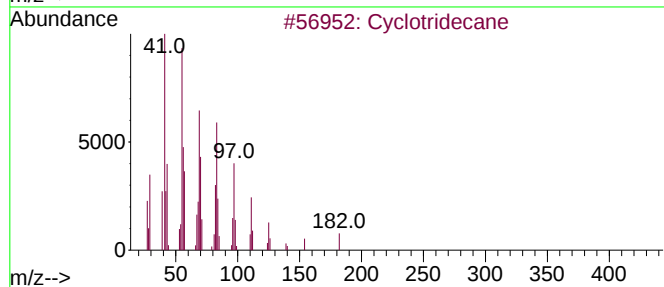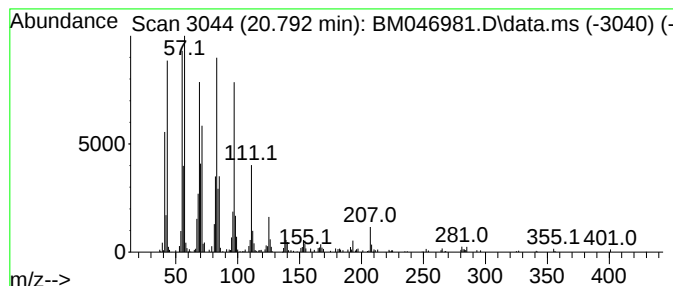

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046981.D
Acq On : 04 Aug 2024 02:10
Operator : MA/JU
Sample : P3276-22
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	20.791	2.7	ng/u1	349716	5	21.050	2588010	20.0