

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080415\
 Data File : BM002232.D
 Acq On : 05 Aug 2015 04:45
 Operator : TP/UM
 Sample : G3095-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01R8RE

Quant Time: Aug 05 05:34:20 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 05 02:56:04 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	163794	20.00	ng/ul	0.01
18) Naphthalene-d8	10.32	136	612549	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	320482	20.00	ng/ul	0.01
62) Phenanthrene-d10	16.97	188	667262	20.00	ng/ul	0.02
78) Chrysene-d12	21.20	240	875908	20.00	ng/ul	0.04
86) Perylene-d12	23.40	264	849865	20.00	ng/ul	0.05

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.96	96	3821	1.33	ng/uL	0.00
5) Phenol-d5	6.73	99	112270	9.23	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	6.86	67	61100	9.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	97427	9.37	ng/ul	0.01
13) 4-Methylphenol-d8	8.26	113	89683	8.87	ng/ul	0.01
19) Nitrobenzene-d5	8.69	128	46215	10.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	51542	9.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	96586	9.64	ng/ul	0.01
29) 4-Chloroaniline-d4	10.47	131	49716	4.48	ng/ul	0.01
44) Dimethylphthalate-d6	13.62	166	254286	10.91	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	320419	10.88	ng/ul	0.01
52) 4-Nitrophenol-d4	14.47	143	29940	9.91	ng/ul	0.02
58) Fluorene-d10	15.20	176	220913	10.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	2238	0.58	ng/ul	0.03
71) Anthracene-d10	17.07	188	328579	11.06	ng/ul	0.02
79) Pyrene-d10	19.39	212	373478	8.91	ng/ul	0.03
90) Benzo(a)pyrene-d12	23.26	264	432447	10.48	ng/ul	0.05

Target Compounds

						Qvalue
28) Naphthalene	10.36	128	122749	4.24	ng/ul	99
34) 2-Methylnaphthalene	11.99	142	41556	1.86	ng/ul	100
35) 1-Methylnaphthalene	12.22	142	39657	1.86	ng/ul	99
45) Dimethylphthalate	13.66	163	76360	3.28	ng/ul	99
48) Acenaphthylene	13.93	152	465332	15.49	ng/ul	99
50) Acenaphthene	14.27	153	189606	9.66	ng/ul	97
54) Dibenzofuran	14.61	168	125788	4.42	ng/ul	98
59) Fluorene	15.26	166	229189	9.80	ng/ul	99
70) Phenanthrene	17.02	178	4306640	125.70	ng/ul	99
72) Anthracene	17.10	178	1171451	33.45	ng/ul	99
75) Carbazole	17.38	167	286177	9.81	ng/ul	99
77) Fluoranthene	19.20	202	190662	5.08	ng/ul	99
80) Pyrene	19.43	202	8426614	156.52	ng/ul#	91
83) Benzo(a)anthracene	21.18	228	5137086	104.69	ng/ul	95
84) Bis(2-ethylhexyl)phthalate	21.09	149	4064124	147.17	ng/ul	96
85) Chrysene	21.18	228	5137086	113.71	ng/ul	97
88) Benzo(b)fluoranthene	22.75	252	5736643	119.80	ng/ul#	96
89) Benzo(k)fluoranthene	22.75	252	1996968	43.06	ng/ul#	97
91) Benzo(a)pyrene	23.32	252	4407952	96.38	ng/ul	97
92) Indeno(1,2,3-cd)pyrene	25.65	276	2840143	55.11	ng/ul	96
93) Dibenzo(a,h)anthracene	25.63	278	801415	18.24	ng/ul#	90
94) Benzo(g,h,i)perylene	26.34	276	2544201	59.28	ng/ul	98

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080415\
Data File : BM002232.D
Acq On : 05 Aug 2015 04:45
Operator : TP/UM
Sample : G3095-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01R8RE

Quant Time: Aug 05 05:34:20 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080415.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 05 02:56:04 2015
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080415\
Data File : BM002232.D
Acq On : 05 Aug 2015 04:45
Operator : TP/UM
Sample : G3095-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01R8RE

Quant Time: Aug 05 05:34:20 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080415.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 05 02:56:04 2015
Response via : Initial Calibration




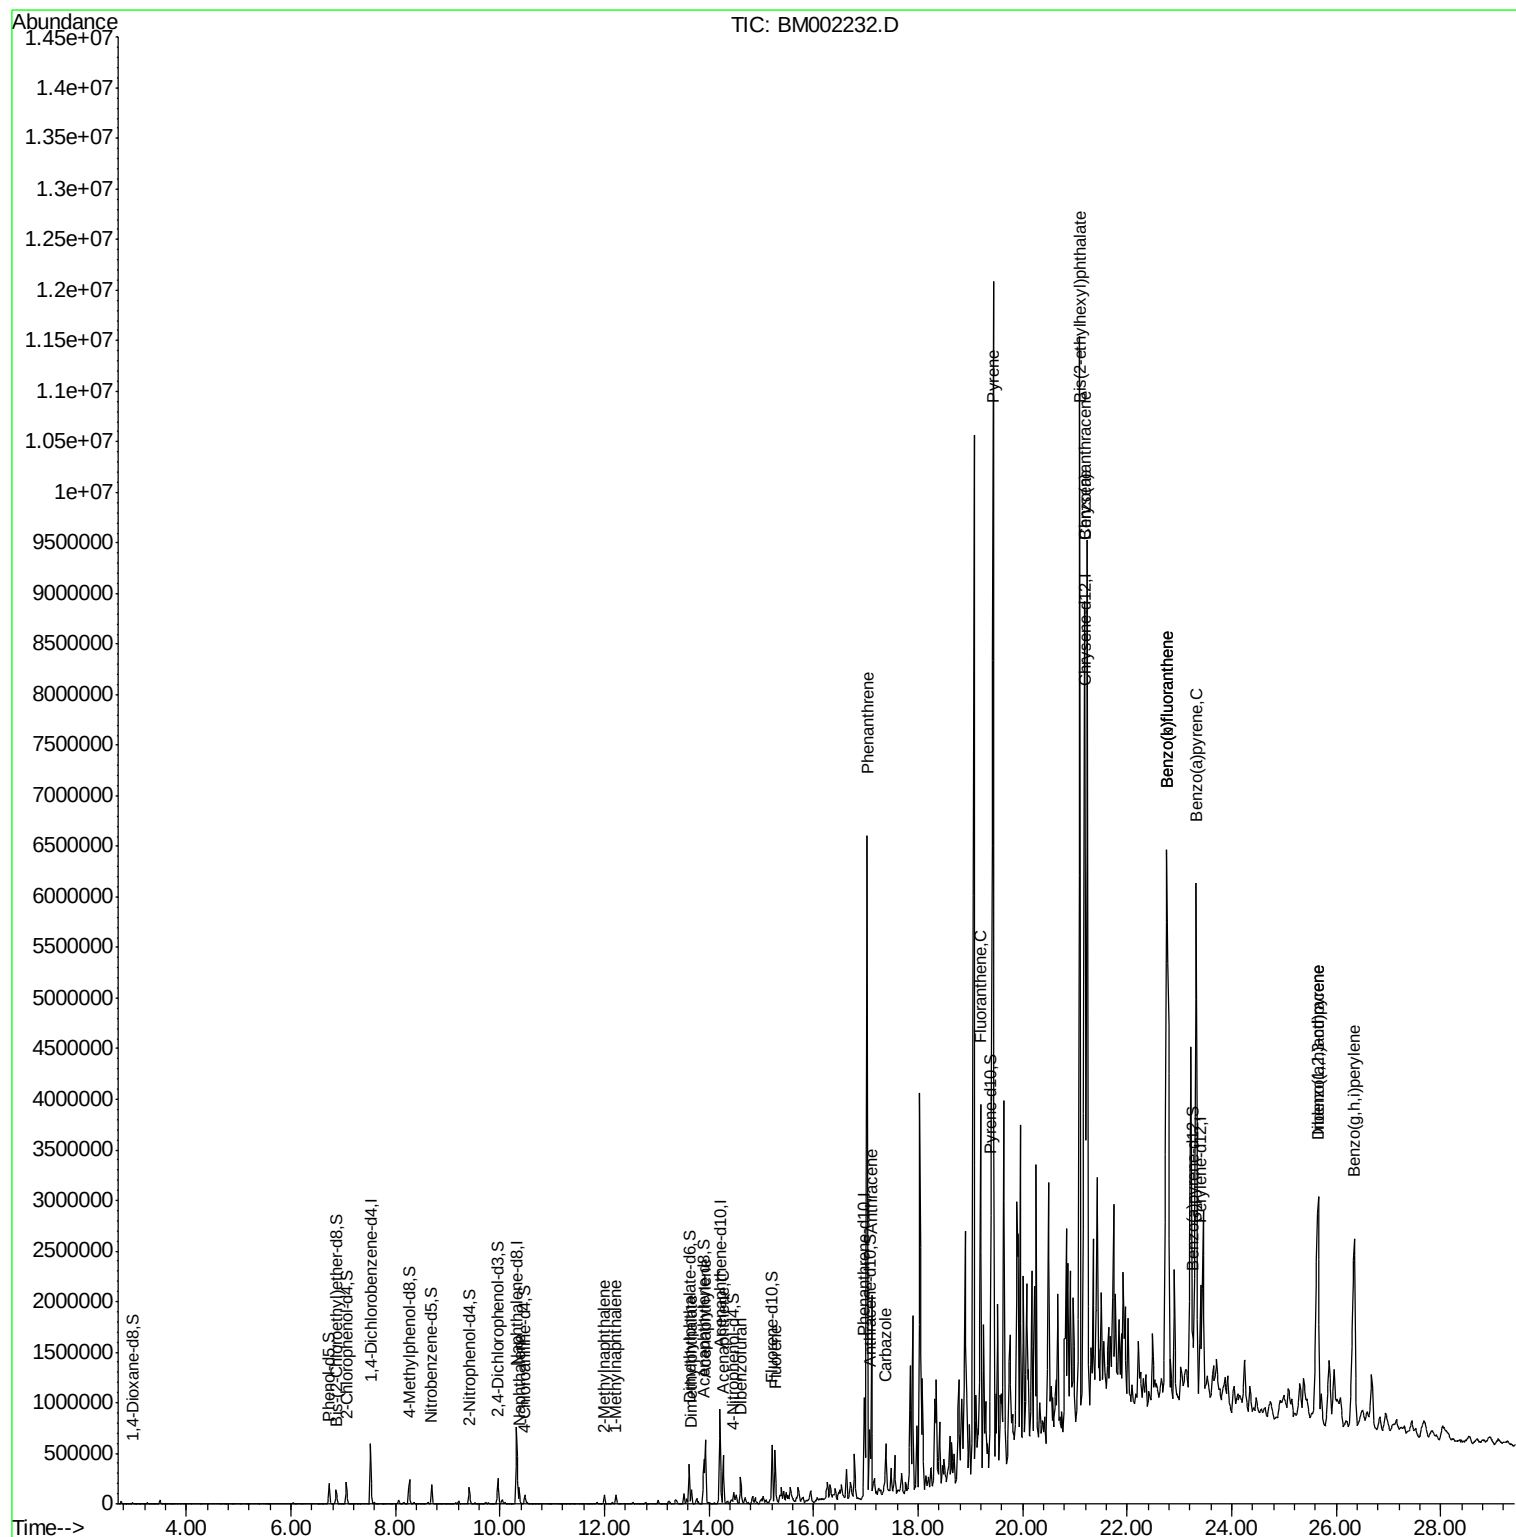


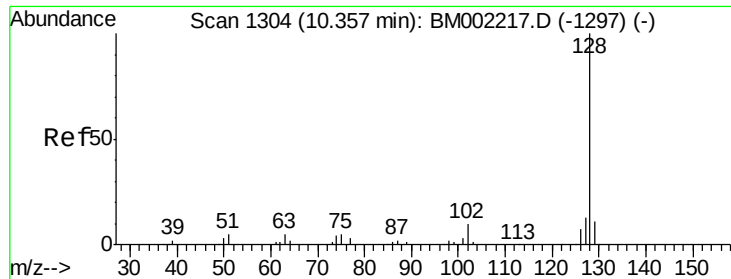

#28
Naphthalene
Concen: 4.24 ng/ul
RT: 10.36 min Scan# 1305
Delta R.T. 0.01 min
Lab File: BM002232.D
Acq: 05 Aug 2015 04:45




Instrument :
BNA_M
ClientSampleId :
C01R8RE


Tgt Ion:128 Resp: 122749
Ion Ratio Lower Upper
128 100
129 10.7 8.2 12.2
127 12.9 10.1 15.1

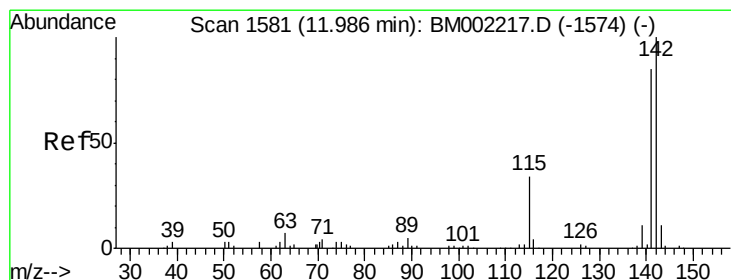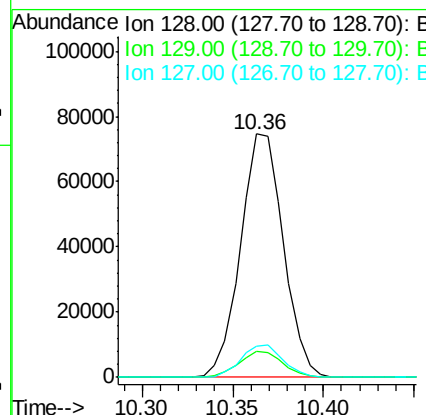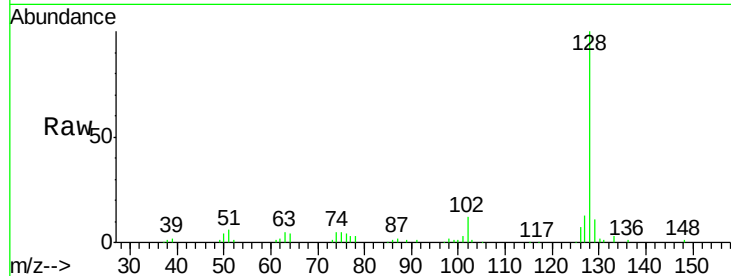

#34
2-Methylnaphthalene
Concen: 1.86 ng/ul
RT: 11.99 min Scan# 1582
Delta R.T. 0.01 min
Lab File: BM002232.D
Acq: 05 Aug 2015 04:45

Tgt Ion:142 Resp: 41556
Ion Ratio Lower Upper
142 100
141 85.8 68.9 103.3

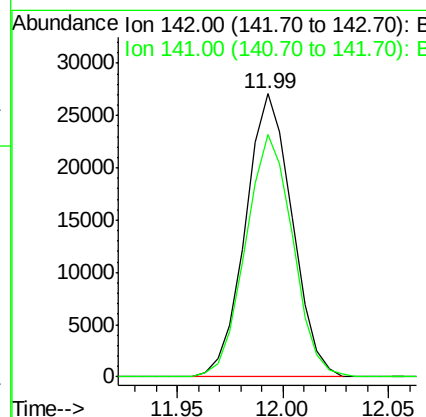

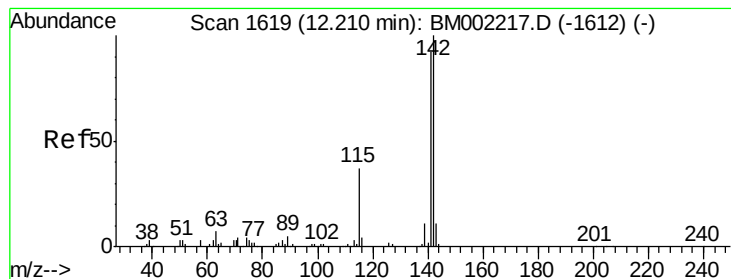

#35

1-Methylnaphthalene

Concen: 1.86 ng/ul

RT: 12.22 min Scan# 1620

Delta R.T. 0.01 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45

Instrument :

BNA_M

ClientSampleId :

C01R8RE


Tgt Ion:142 Resp: 39657

Ion Ratio Lower Upper

142 100

141 89.7 71.0 106.4




116 4.1 3.3 4.9



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

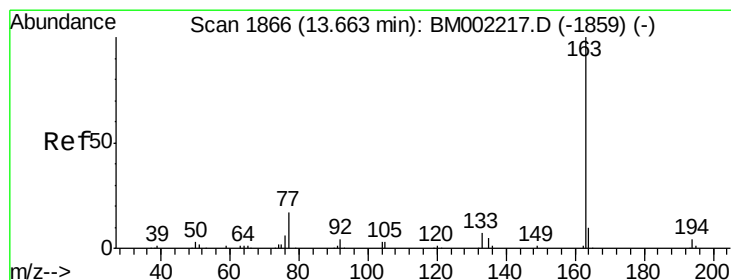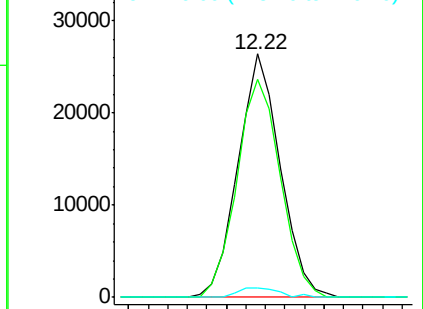

#45

Dimethylphthalate

Concen: 3.28 ng/ul

RT: 13.66 min Scan# 1866

Delta R.T. 0.00 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45


Tgt Ion:163 Resp: 76360

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2



164 10.3 7.9 11.9




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

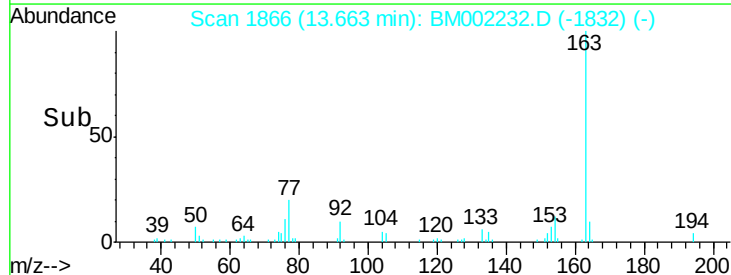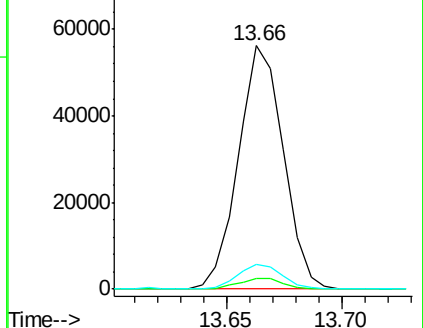

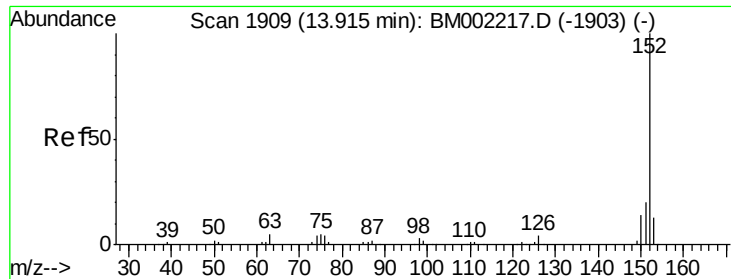

#48

Acenaphthylene

Concen: 15.49 ng/ul

RT: 13.93 min Scan# 1911

Delta R.T. 0.01 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45

Instrument :

BNA_M

ClientSampleId :

C01R8RE


Tgt Ion:152 Resp: 465332

Ion Ratio Lower Upper

152 100

151 19.1 15.2 22.8




153 13.4 10.3 15.5

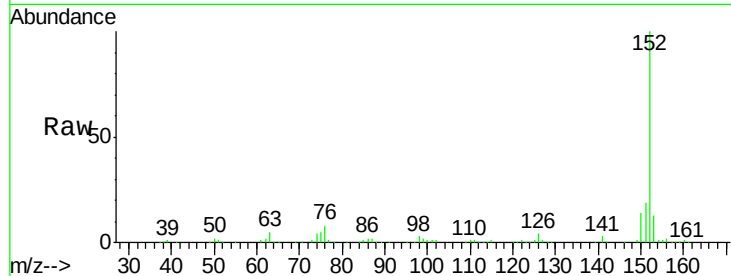

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

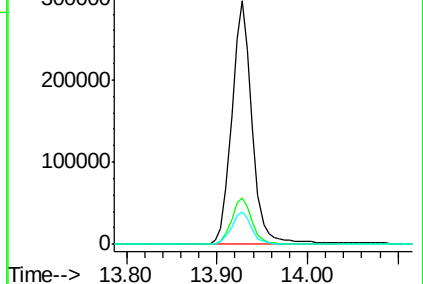

#50

Acenaphthene

Concen: 9.66 ng/ul

RT: 14.27 min Scan# 1969

Delta R.T. 0.01 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45


Tgt Ion:153 Resp: 189606

Ion Ratio Lower Upper

153 100

152 46.7 36.6 54.8



154 92.6 71.7 107.5




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

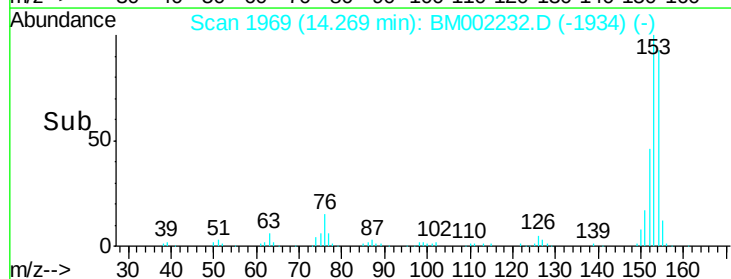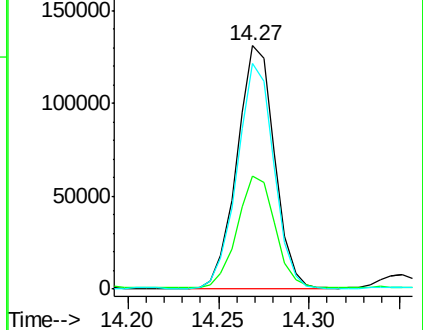

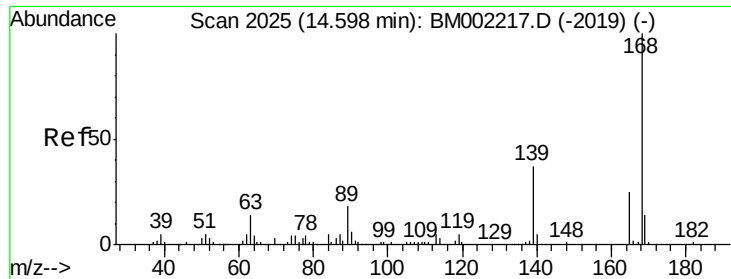

#54

Dibenzenofuran

Concen: 4.42 ng/ul

RT: 14.61 min Scan# 2027

Delta R.T. 0.01 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45

Instrument :

BNA_M

ClientSampleId :


C01R8RE

Tgt Ion:168 Resp: 125788

Ion Ratio Lower Upper




168 100

139 34.6 28.6 42.8

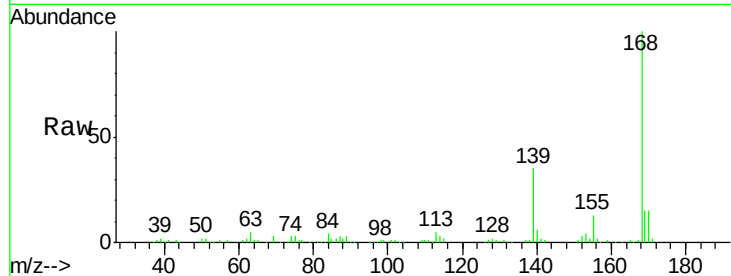

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

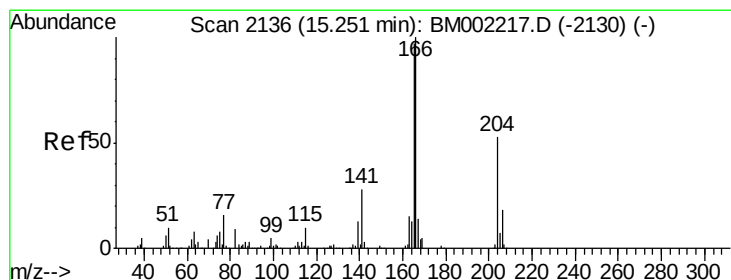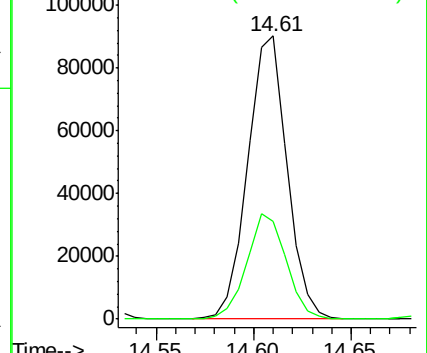

#59

Fluorene

Concen: 9.80 ng/ul

RT: 15.26 min Scan# 2138

Delta R.T. 0.01 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45


Tgt Ion:166 Resp: 229189

Ion Ratio Lower Upper

166 100

165 95.9 76.0 114.0



167 14.2 10.5 15.7




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

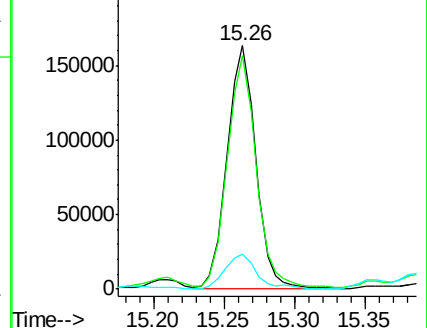



#70

Phenanthrene

Concen: 125.70 ng/ul

RT: 17.02 min Scan# 2437

Delta R.T. 0.02 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45

Instrument :

BNA_M

ClientSampleId :

C01R8RE


Tgt Ion:178 Resp: 4306640

Ion Ratio Lower Upper

178 100

179 15.8 12.2 18.4




176 18.8 14.6 21.8



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

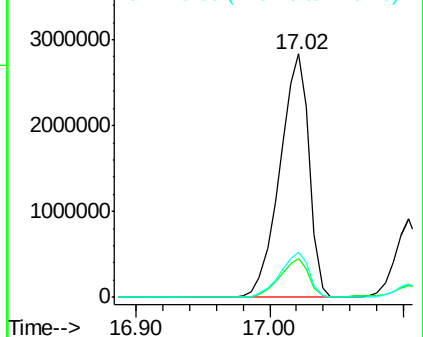

#72

Anthracene

Concen: 33.45 ng/ul

RT: 17.10 min Scan# 2451

Delta R.T. 0.02 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45


Tgt Ion:178 Resp: 1171451

Ion Ratio Lower Upper

178 100

179 15.4 12.2 18.2



176 17.5 13.8 20.6




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

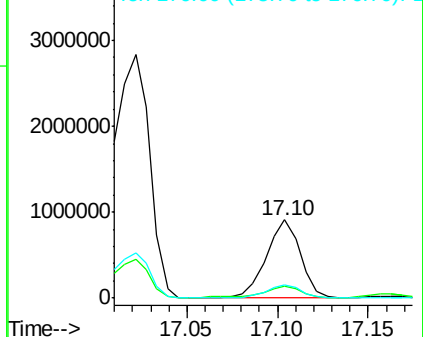



#75

Carbazole

Concen: 9.81 ng/ul

RT: 17.38 min Scan# 2498

Delta R.T. 0.02 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45

Instrument :

BNA_M

ClientSampleId :

C01R8RE


Tgt Ion:167 Resp: 286177

Ion Ratio Lower Upper

167 100

166 21.2 16.7 25.1




139 12.6 9.4 14.2



Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

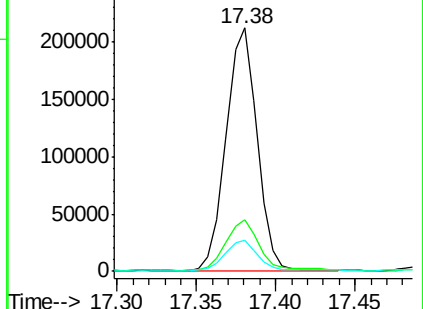

#77

Fluoranthene

Concen: 5.08 ng/ul

RT: 19.20 min Scan# 2807

Delta R.T. 0.18 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45


Tgt Ion:202 Resp: 190662

Ion Ratio Lower Upper

202 100

101 7.7 6.2 9.2



100 6.6 4.8 7.2




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

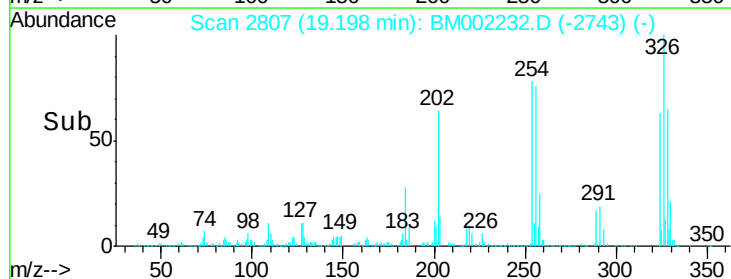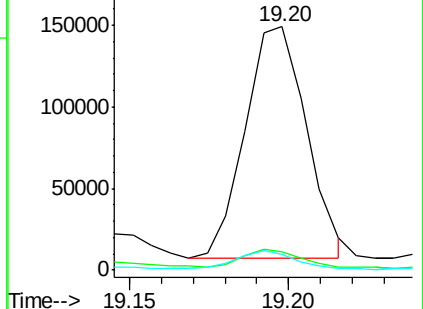

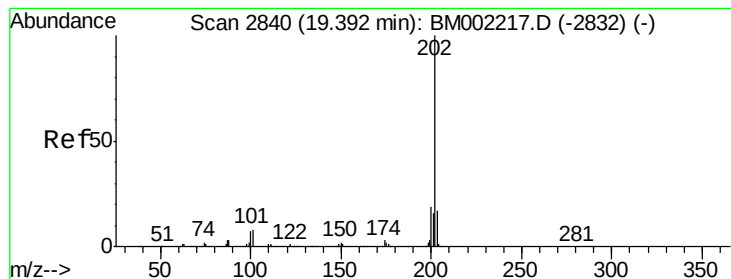

#80

Pyrene

Concen: 156.52 ng/ul

RT: 19.43 min Scan# 2847

Delta R.T. 0.04 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45

Instrument :

BNA_M

ClientSampleId :

C01R8RE


Tgt Ion:202 Resp: 8426614

Ion Ratio Lower Upper

202 100

101 12.4 7.0 10.6#




100 10.3 5.8 8.8#



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

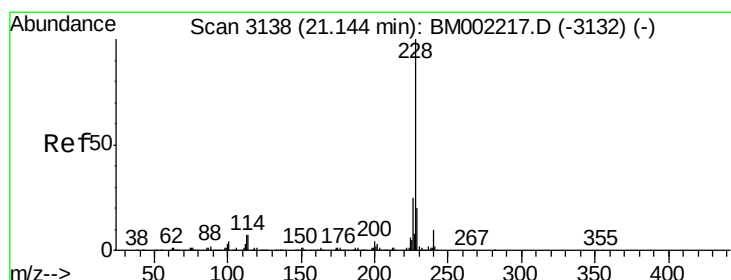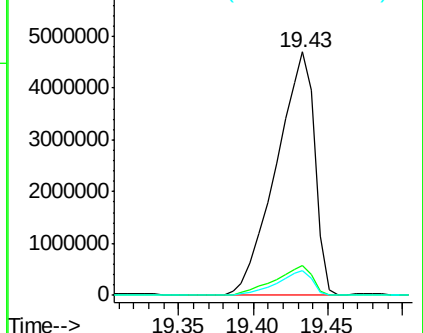

#83

Benzo(a)anthracene

Concen: 104.69 ng/ul

RT: 21.18 min Scan# 3144

Delta R.T. 0.04 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45


Tgt Ion:228 Resp: 5137086

Ion Ratio Lower Upper

228 100

229 21.4 15.9 23.9



226 29.2 20.6 31.0




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

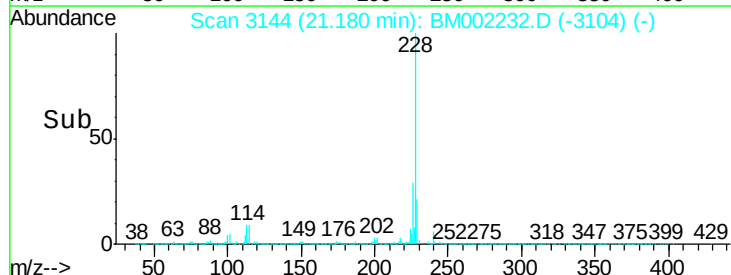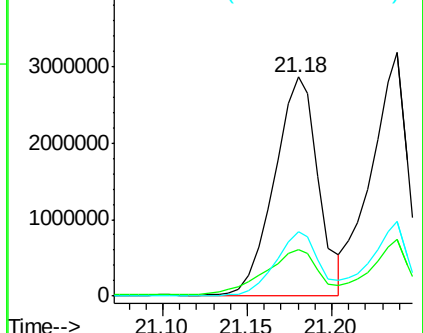

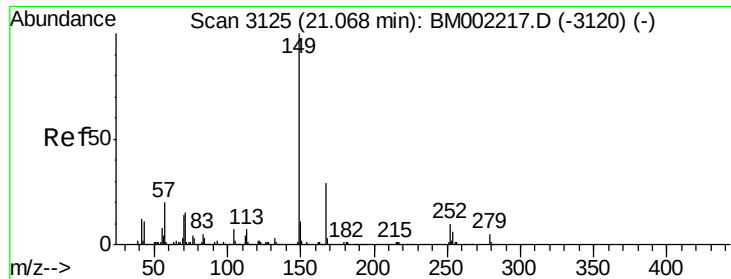

#84

Bis(2-ethylhexyl)phthalate

Concen: 147.17 ng/ul

RT: 21.09 min Scan# 3129

Delta R.T. 0.02 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45

Instrument :

BNA_M

ClientSampleId :

C01R8RE


Tgt Ion:149 Resp: 4064124

Ion Ratio Lower Upper

149 100

167 30.7 23.0 34.4




279 5.7 4.0 6.0

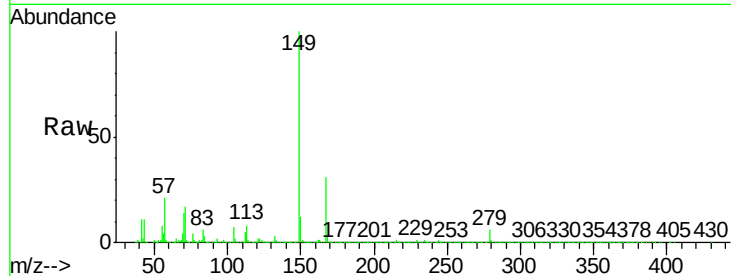

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

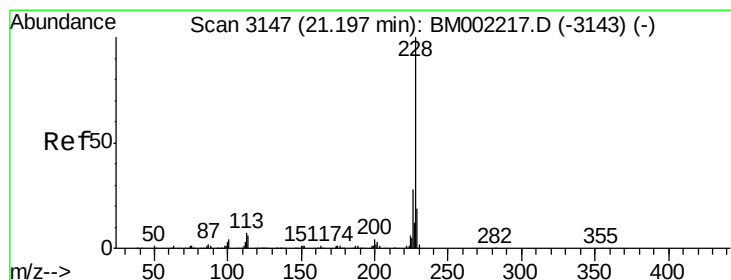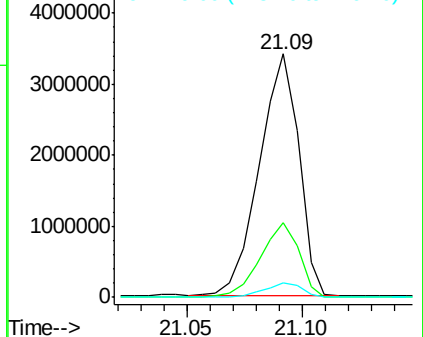

#85

Chrysene

Concen: 113.71 ng/ul

RT: 21.18 min Scan# 3144

Delta R.T. -0.02 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45


Tgt Ion:228 Resp: 5137086

Ion Ratio Lower Upper

228 100

226 29.2 22.2 33.4



229 21.4 15.5 23.3




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E




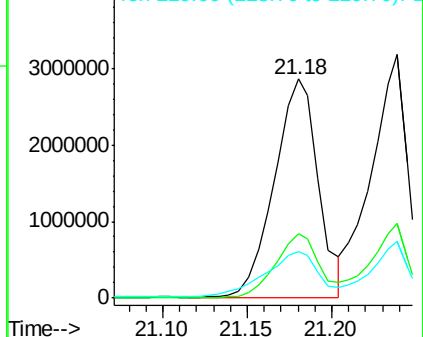


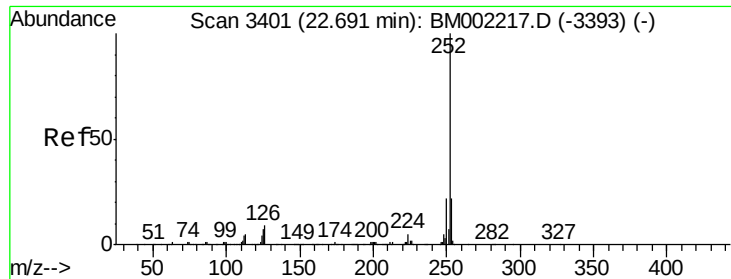

#88
Benzo(b)fluoranthene
Concen: 119.80 ng/ul
RT: 22.75 min Scan# 3411
Delta R.T. 0.06 min
Lab File: BM002232.D
Acq: 05 Aug 2015 04:45




Instrument :
BNA_M
ClientSampleId :
C01R8RE


Tgt Ion:252 Resp: 5736643
Ion Ratio Lower Upper
252 100
253 22.9 17.4 26.0
125 9.2 5.4 8.2#

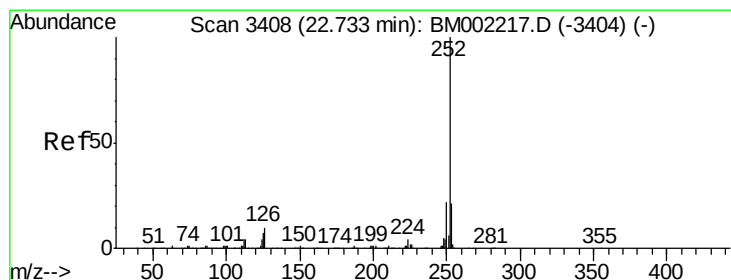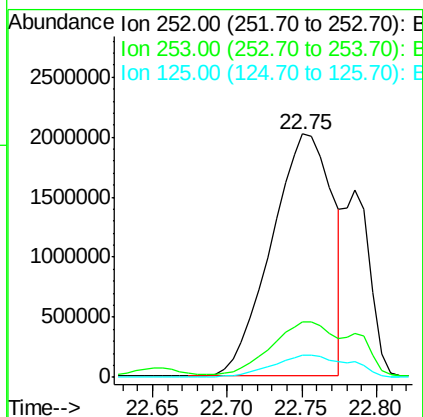

#89
Benzo(k)fluoranthene
Concen: 43.06 ng/ul
RT: 22.75 min Scan# 3411
Delta R.T. 0.02 min
Lab File: BM002232.D
Acq: 05 Aug 2015 04:45

Tgt Ion:252 Resp: 1996968
Ion Ratio Lower Upper
252 100
253 22.9 17.4 26.2
125 9.2 5.6 8.4#

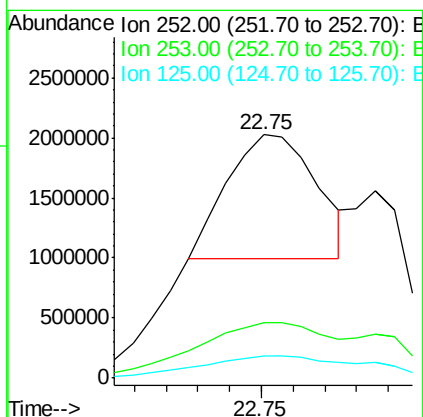

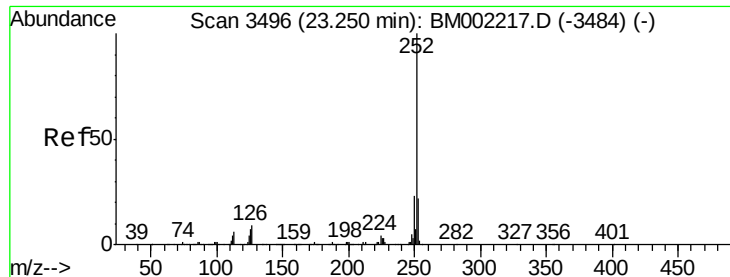

#91

Benzo(a)pyrene

Concen: 96.38 ng/ul

RT: 23.32 min Scan# 3508

Delta R.T. 0.07 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45

Instrument :

BNA_M

ClientSampleId :

C01R8RE


Tgt Ion:252 Resp: 4407952

Ion Ratio Lower Upper

252 100

253 23.2 17.4 26.0




125 9.1 6.1 9.1

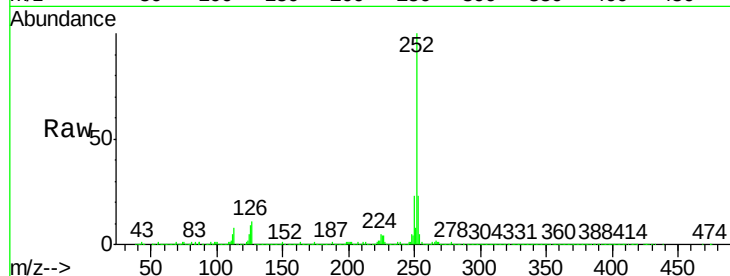

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

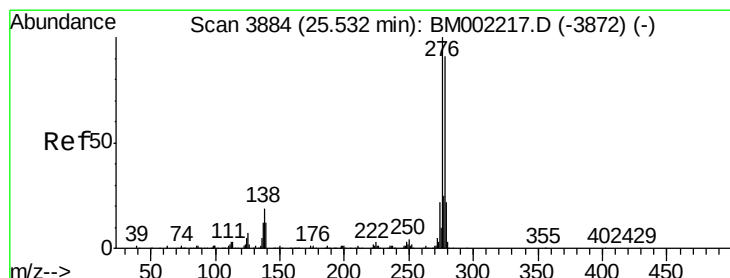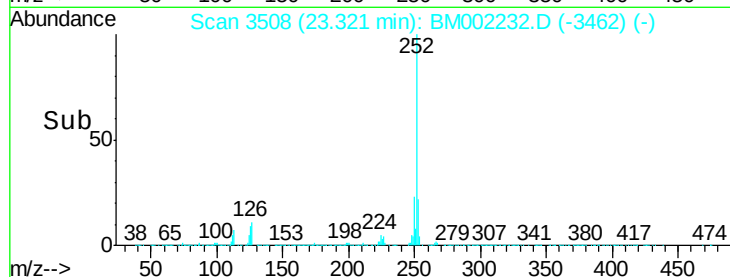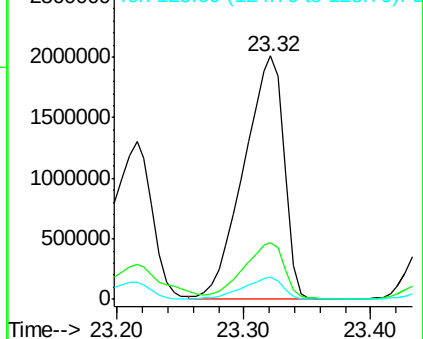

#92

Indeno(1,2,3-cd)pyrene

Concen: 55.11 ng/ul

RT: 25.65 min Scan# 3904

Delta R.T. 0.12 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45


Tgt Ion:276 Resp: 2840143

Ion Ratio Lower Upper

276 100

138 16.1 15.4 23.0



277 24.5 20.2 30.2

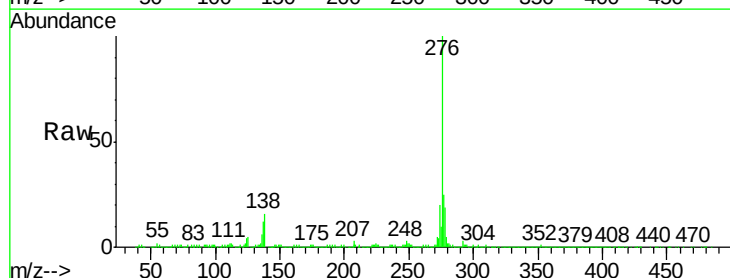


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

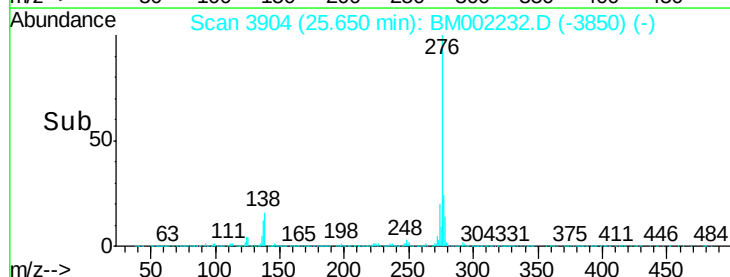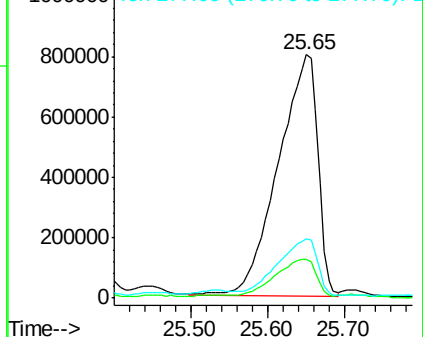

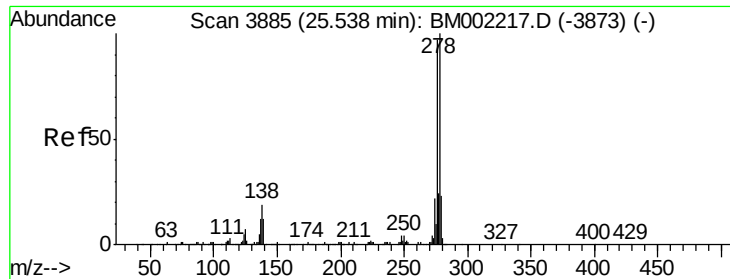

#93

Dibenzo(a,h)anthracene

Concen: 18.24 ng/ul

RT: 25.63 min Scan# 3901

Delta R.T. 0.09 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45

Instrument :

BNA_M

ClientSampleId :

C01R8RE


Tgt Ion:278 Resp: 801415

Ion Ratio Lower Upper

278 100

139 15.1 10.4 15.6




279 28.8 17.9 26.9#

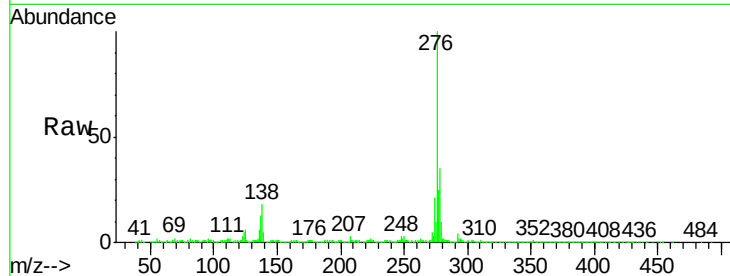

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

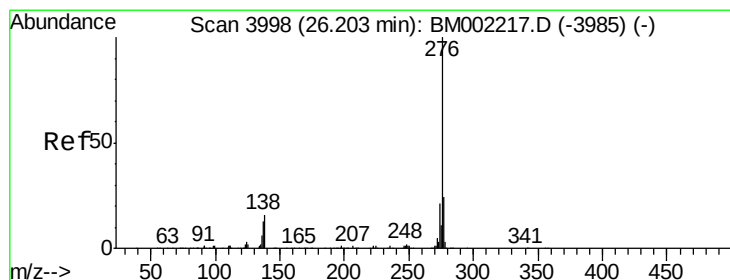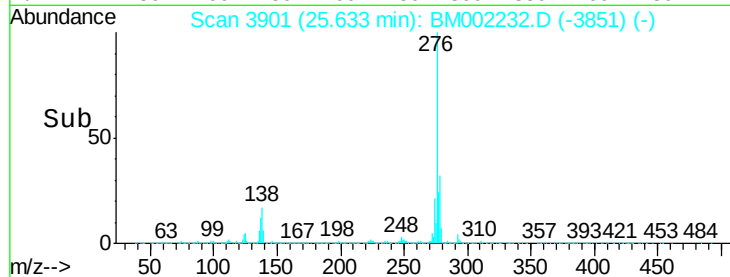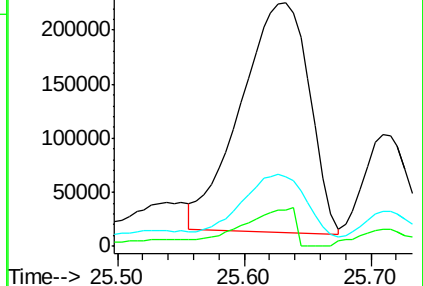

#94

Benzo(g,h,i)perylene

Concen: 59.28 ng/ul

RT: 26.34 min Scan# 4021

Delta R.T. 0.14 min

Lab File: BM002232.D

Acq: 05 Aug 2015 04:45


Tgt Ion:276 Resp: 2544201

Ion Ratio Lower Upper

276 100

138 16.7 12.5 18.7

277 24.8 19.4 29.0

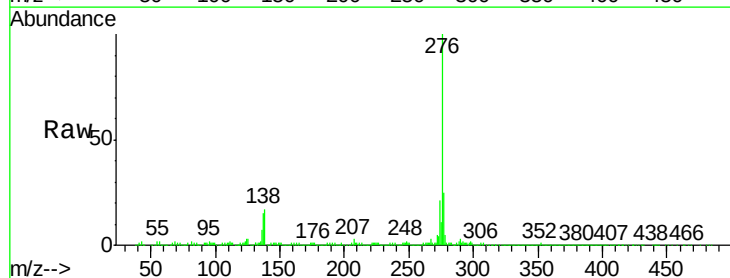

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

