


Data Path : Z:\HPCHEM1\BNA_M\Data\BM080415\
Data File : BM002210.D
Acq On : 04 Aug 2015 12:35
Operator : TP/UM
Sample : DFTPP89
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP89

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080415.M
Title : SVOA CALIBRATION
Last Update : Thu Aug 06 01:44:45 2015

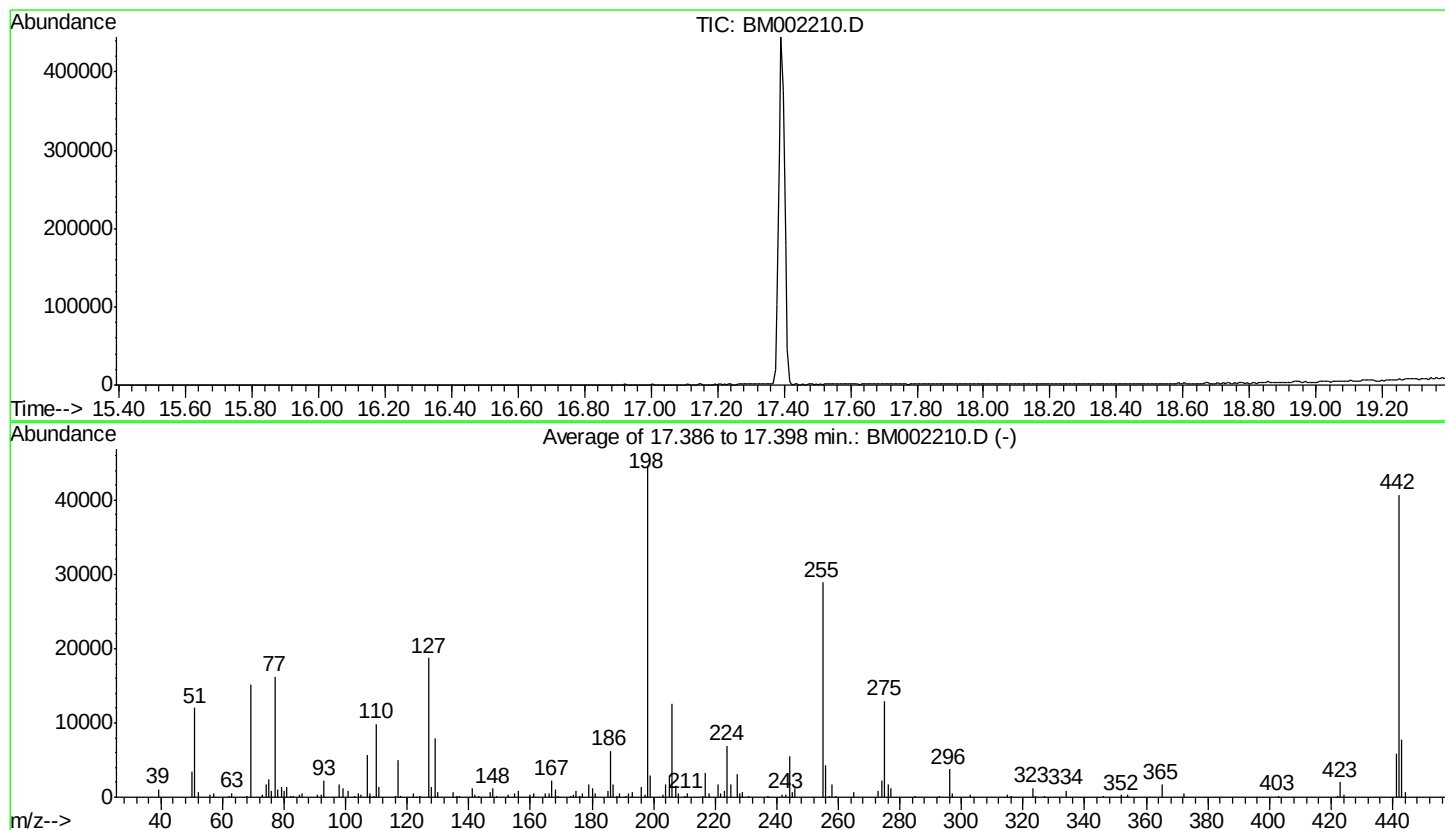

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	11990	PASS
68	69	0.00	2	1.5	227	PASS
69	198	0.00	100	34.0	15175	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.9	18714	PASS
197	198	0.00	2	0.7	321	PASS
198	198	100	100	100.0	44613	PASS
199	198	5	9	6.8	3015	PASS
275	198	10	60	29.2	13007	PASS
365	198	1	100	3.8	1698	PASS
441	443	0.01	100	75.8	5941	PASS
442	198	50	100	91.1	40656	PASS
443	442	15	24	19.3	7835	PASS

Scan 2494 (17.356 min): BM002210.D
DFTPP89

m/z	Abundance
41.10	320.0
44.00	518.0
57.00	334.0
123.00	650.0
207.00	504.0

Instrument :
BNA_M
ClientSampleId :
DFTPP89

m/z	Abundance
39.00	937.0
43.90	363.0
50.10	3226.0
51.00	12005.0
52.00	675.0
55.90	363.0
57.00	843.0
63.00	601.0
68.10	308.0
69.00	14689.0
73.00	300.0
74.00	1547.0
74.90	2270.0
76.00	763.0
77.00	15549.0
78.00	991.0
79.00	1397.0
79.90	819.0
81.00	1479.0
83.00	336.0
85.00	308.0
86.00	488.0
91.90	303.0
93.00	1974.0
98.00	1529.0
99.00	1129.0
100.90	806.0
104.00	516.0
104.90	497.0
107.00	4825.0
107.90	786.0
110.00	8821.0
110.90	1363.0
117.00	4556.0
121.90	448.0
123.00	543.0
127.00	16696.0
128.00	1120.0
129.00	6852.0
130.00	528.0
135.00	556.0
141.00	1083.0
141.90	409.0
146.90	511.0
148.00	1209.0
152.90	321.0
155.00	522.0
156.10	633.0
160.90	519.0
165.00	392.0
166.10	427.0
166.90	2046.0
168.00	785.0
175.00	810.0
176.80	424.0
178.90	1313.0
180.00	1048.0
181.00	452.0
185.00	775.0
186.00	5289.0
186.90	1490.0
188.90	348.0
191.90	587.0
193.10	578.0
196.00	1194.0
197.90	36728.0
198.90	2353.0
202.80	329.0
204.00	1353.0
205.00	2296.0
206.00	10174.0
207.00	1905.0
207.90	345.0
210.80	386.0
216.90	2736.0
217.90	352.0
221.10	1362.0
221.90	412.0
223.00	809.0
224.00	5163.0
225.00	1397.0
227.00	2625.0
227.90	384.0
229.00	536.0
243.00	356.0
244.00	4261.0
245.00	645.0
246.00	793.0
255.00	22696.0
256.00	3209.0
258.00	1236.0

Instrument :
BNA_M
ClientSampleId :
DFTPP89

265.00	537.0
273.00	703.0
274.00	1644.0
275.00	9294.0
276.00	1208.0
277.00	899.0
296.00	2771.0
297.00	403.0
302.90	310.0
323.00	859.0
334.10	673.0
354.00	414.0
364.90	1101.0
372.10	377.0
423.00	1254.0
441.00	3473.0
442.00	24504.0
443.00	4819.0
444.00	399.0

Instrument :
BNA_M
ClientSampleId :
DFTPP89

m/z	Abundance
39.10	1118.0
44.00	457.0
50.00	3990.0
51.10	14083.0
52.10	725.0
56.00	476.0
57.00	1008.0
62.00	360.0
63.10	701.0
68.10	375.0
69.00	17800.0
72.90	428.0
74.00	1931.0
75.00	3028.0
76.00	1046.0
77.00	19096.0
78.00	1300.0
79.00	1753.0
80.00	1120.0
81.00	1426.0
83.00	381.0
85.00	412.0
85.90	526.0
91.00	542.0
91.90	395.0
93.00	2593.0
98.00	2257.0
99.00	1745.0
100.90	855.0
102.90	352.0
103.90	563.0
104.90	603.0
107.00	6827.0
108.10	892.0
110.00	11757.0
111.00	1689.0
116.00	396.0
117.00	6185.0
118.00	526.0
121.90	506.0
123.00	857.0
123.90	360.0
127.00	22440.0
128.00	1474.0
129.00	9433.0
129.90	794.0
135.00	728.0
136.00	344.0
137.00	378.0
141.00	1395.0
141.90	410.0
147.00	678.0
148.00	1441.0
148.90	344.0
152.90	458.0
155.00	649.0
155.90	1042.0
160.00	508.0
161.00	569.0
164.90	524.0
166.00	516.0
167.00	2669.0
167.90	1402.0
168.90	319.0
173.00	321.0
173.90	548.0
175.00	979.0
176.10	332.0
176.90	656.0
179.00	1998.0
180.10	1342.0
181.00	595.0
185.00	859.0
186.00	7059.0
187.00	2148.0
188.10	370.0
189.00	681.0
191.00	311.0
192.00	649.0
193.00	724.0
196.00	1390.0
197.10	483.0
197.90	52712.0
198.90	3646.0
202.90	478.0
204.00	2165.0
205.00	3517.0
206.00	15238.0
207.00	2340.0
208.00	704.0
210.00	306.0

Instrument :
BNA_M
ClientSampleId :
DFTPP89

210.90	574.0
215.90	331.0
217.00	3716.0
218.00	577.0
221.10	1962.0
221.90	475.0
223.00	1088.0
224.00	8473.0
225.00	1998.0
227.00	3686.0
227.90	491.0
229.00	736.0
231.00	352.0
242.00	468.0
243.00	449.0
244.00	6305.0
245.00	914.0
246.00	1461.0
255.00	33928.0
256.00	5230.0
256.90	408.0
258.00	2197.0
259.00	313.0
264.90	716.0
272.90	996.0
274.00	2766.0
275.00	15489.0
276.00	2134.0
276.90	1512.0
284.90	398.0
292.90	322.0
296.00	4396.0
297.00	560.0
303.00	435.0
314.90	360.0
316.00	310.0
323.00	1566.0
324.10	301.0
334.00	1000.0
352.00	499.0
365.00	2019.0
372.00	585.0
402.90	362.0
422.00	325.0
423.10	2476.0
424.10	498.0
441.10	6822.0
442.10	47024.0
443.10	9304.0
444.00	894.0

Instrument :
BNA_M
ClientSampleId :
DFTPP89

m/z	Abundance
39.00	1050.0
44.00	430.0
50.00	2962.0
51.10	9883.0
52.00	491.0
56.00	380.0
57.00	949.0
63.00	420.0
69.00	13037.0
72.90	359.0
74.00	1494.0
75.00	2102.0
76.00	827.0
77.00	14065.0
78.00	818.0
79.00	1122.0
79.90	908.0
81.00	1244.0
82.00	323.0
85.00	314.0
85.90	373.0
91.00	326.0
92.00	369.0
93.00	2017.0
98.00	1485.0
99.00	960.0
101.00	792.0
103.90	505.0
107.00	5274.0
108.00	766.0
108.90	322.0
110.00	8880.0
111.00	1276.0
116.00	330.0
117.00	4456.0
121.90	403.0
123.00	646.0
124.00	328.0
127.00	17008.0
128.00	1410.0
129.00	7470.0
129.90	587.0
135.00	680.0
140.90	1013.0
143.00	322.0
147.00	729.0
147.90	956.0
152.90	359.0
155.00	536.0
156.10	803.0
159.90	350.0
161.00	640.0
165.10	505.0
165.90	395.0
167.00	1815.0
168.00	792.0
173.90	452.0
174.90	855.0
176.00	347.0
176.90	431.0
178.90	1695.0
179.90	1100.0
181.00	627.0
185.10	843.0
186.00	6360.0
186.90	1669.0
188.90	318.0
191.90	519.0
193.00	849.0
195.90	1414.0
197.10	480.0
198.00	44400.0
198.90	3046.0
203.00	377.0
204.00	1853.0
205.00	3018.0
206.00	12222.0
207.00	2102.0
208.00	652.0
211.00	565.0
216.90	3541.0
218.00	410.0
221.00	1915.0
221.90	459.0
223.00	727.0
224.00	7067.0
225.00	1637.0
227.00	3248.0
227.90	519.0
228.90	673.0
231.00	425.0

Instrument :
BNA_M
ClientSampleId :
DFTPP89

237.10	345.0
241.80	333.0
243.10	401.0
244.00	5805.0
245.00	733.0
246.00	1270.0
255.00	30040.0
256.00	4560.0
256.90	301.0
258.00	1878.0
264.90	710.0
273.00	1023.0
274.00	2384.0
275.00	14238.0
276.00	1645.0
276.90	1311.0
296.00	4122.0
296.90	525.0
303.10	425.0
315.00	521.0
323.00	1214.0
324.00	311.0
326.90	375.0
334.00	1039.0
346.00	364.0
352.00	352.0
354.00	420.0
365.00	1974.0
372.00	594.0
403.00	359.0
422.10	302.0
423.10	2240.0
424.00	488.0
441.00	7530.0
442.00	50440.0
443.10	9382.0
444.00	895.0

Instrument :
BNA_M
ClientSampleId :
DFTPP89