

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080416\
 Data File : BM006875.D
 Acq On : 04 Aug 2016 22:09
 Operator : UM/SJ
 Sample : H4095-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJH1

Manual Integrations
 APPROVED

umangi
 8/5/2016 7:01:03 PM

Quant Time: Aug 05 04:53:14 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM080316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 05 02:18:21 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	234563	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	951940	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	590408	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	1412615	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	1573516	20.00	ng/ul	0.00
83) Perylene-d12	23.37	264	1400558	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	5120m	1.20	ng/uL	0.00
5) Phenol-d5	6.80	99	188511	10.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	137786	11.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	168844	12.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	147407	10.50	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	76767	11.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	86928	11.22	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.02	165	177120m	11.06	ng/ul	0.01
29) 4-Chloroaniline-d4	10.53	131	196854	11.89	ng/ul	0.01
43) Dimethylphthalate-d6	13.65	166	648357	13.33	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	754617	12.71	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	58761m	5.51	ng/ul	0.04
57) Fluorene-d10	15.22	176	581566	12.88	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	48070m	5.21	ng/ul	0.01
70) Anthracene-d10	17.07	188	904614	13.33	ng/ul	0.00
76) Pyrene-d10	19.38	212	1096940	13.63	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.23	264	913869m	13.40	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	13.69	163	380065	7.86 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM080416\
Data File : BM006875.D
Acq On : 04 Aug 2016 22:09
Operator : UM/SJ
Sample : H4095-16
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BDJH1

Manual Integrations
APPROVED

umangi
8/5/2016 7:01:03 PM

Quant Time: Aug 05 04:53:14 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 05 02:18:21 2016
Response via : Initial Calibration

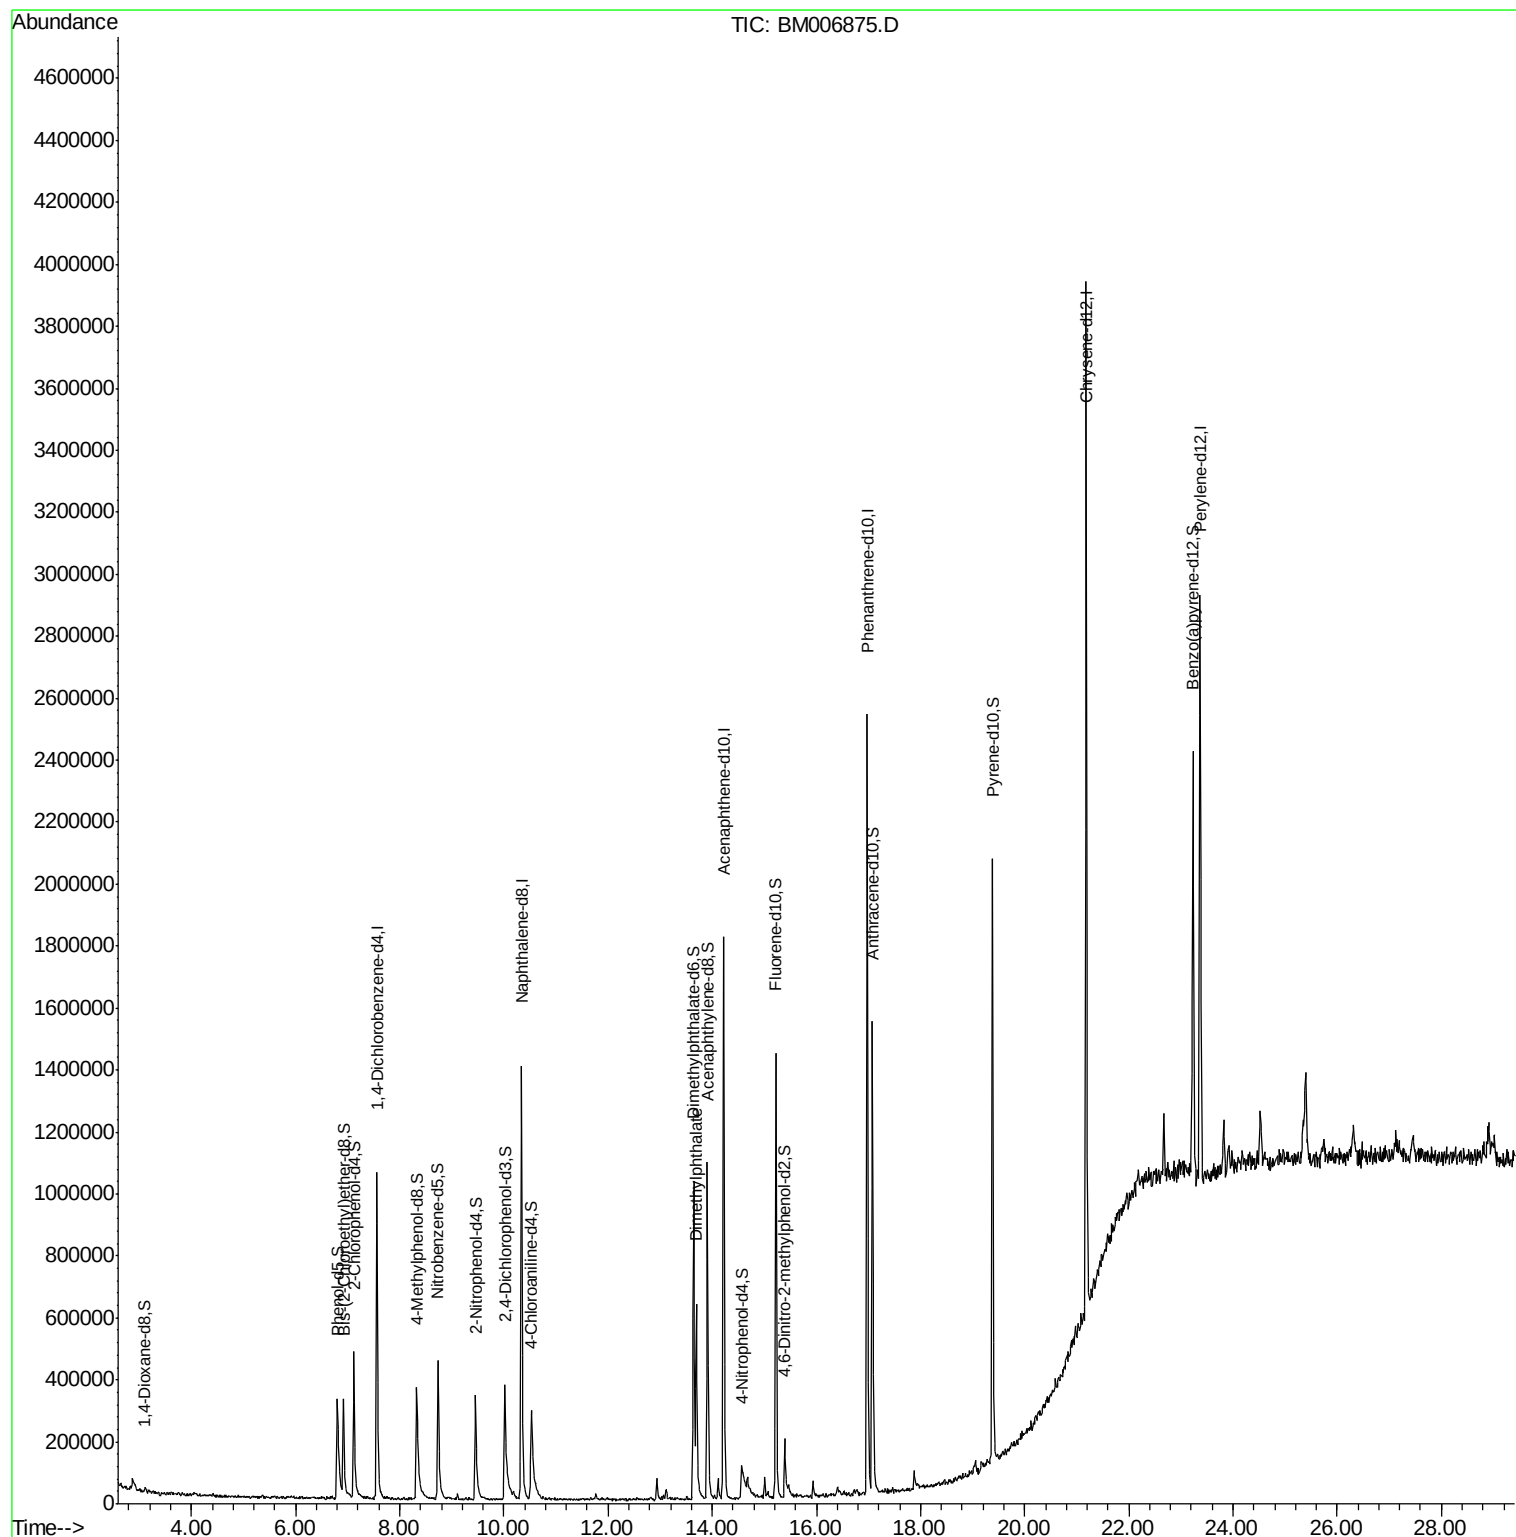

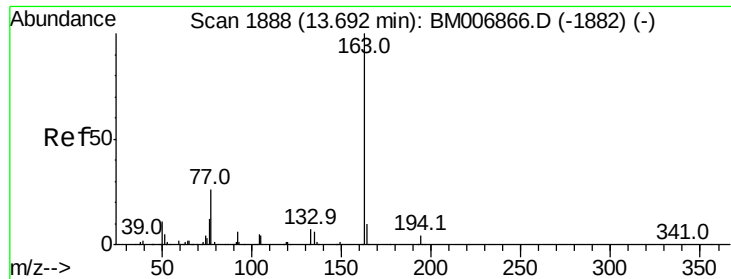

#44
 Dimethylphthalate
 Concen: 7.86 ng/ul
 RT: 13.69 min Scan# 1888
 Delta R.T. -0.01 min
 Lab File: BM006875.D
 Acq: 04 Aug 2016 22:09

Instrument :
 BNA_M
 ClientSampleId :
 BDJH1

Tot Ion:	163	Resp:	380065
Ion Ratio	Lower	Upper	
163	100		
194	3.9	3.1	4.7
164	9.5	8.6	12.8

Manual Integrations
 APPROVED

umangi
 8/5/2016 7:01:03 PM

