

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080416\
 Data File : BM006877.D
 Acq On : 04 Aug 2016 23:21
 Operator : UM/SJ
 Sample : H4095-18
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJH3

Manual Integrations
 APPROVED

umangi
 8/5/2016 7:01:20 PM

Quant Time: Aug 05 04:58:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM080316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 05 02:18:21 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	261740	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	1127156	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	744923	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	1794735	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	2014142	20.00	ng/ul	0.00
83) Perylene-d12	23.37	264	1765689	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.11	96	9599m	2.02	ng/uL	0.00
5) Phenol-d5	6.79	99	414667	21.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	294411	22.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	351600	23.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	349067	22.28	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	165725	21.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	195038	21.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	354870	18.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	456147m	23.28	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	1433944	23.37	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	1626040	21.70	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	139568m	10.37	ng/ul	0.00
57) Fluorene-d10	15.22	176	1235740	21.70	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	143045	12.21	ng/ul	0.00
70) Anthracene-d10	17.07	188	1947943	22.60	ng/ul	0.00
76) Pyrene-d10	19.38	212	2329276	22.61	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.23	264	2058513	23.94	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.69	163	892656	14.64	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM080416\
Data File : BM006877.D
Acq On : 04 Aug 2016 23:21
Operator : UM/SJ
Sample : H4095-18
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BDJH3

Quant Time: Aug 05 04:58:42 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 05 02:18:21 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
8/5/2016 7:01:20 PM

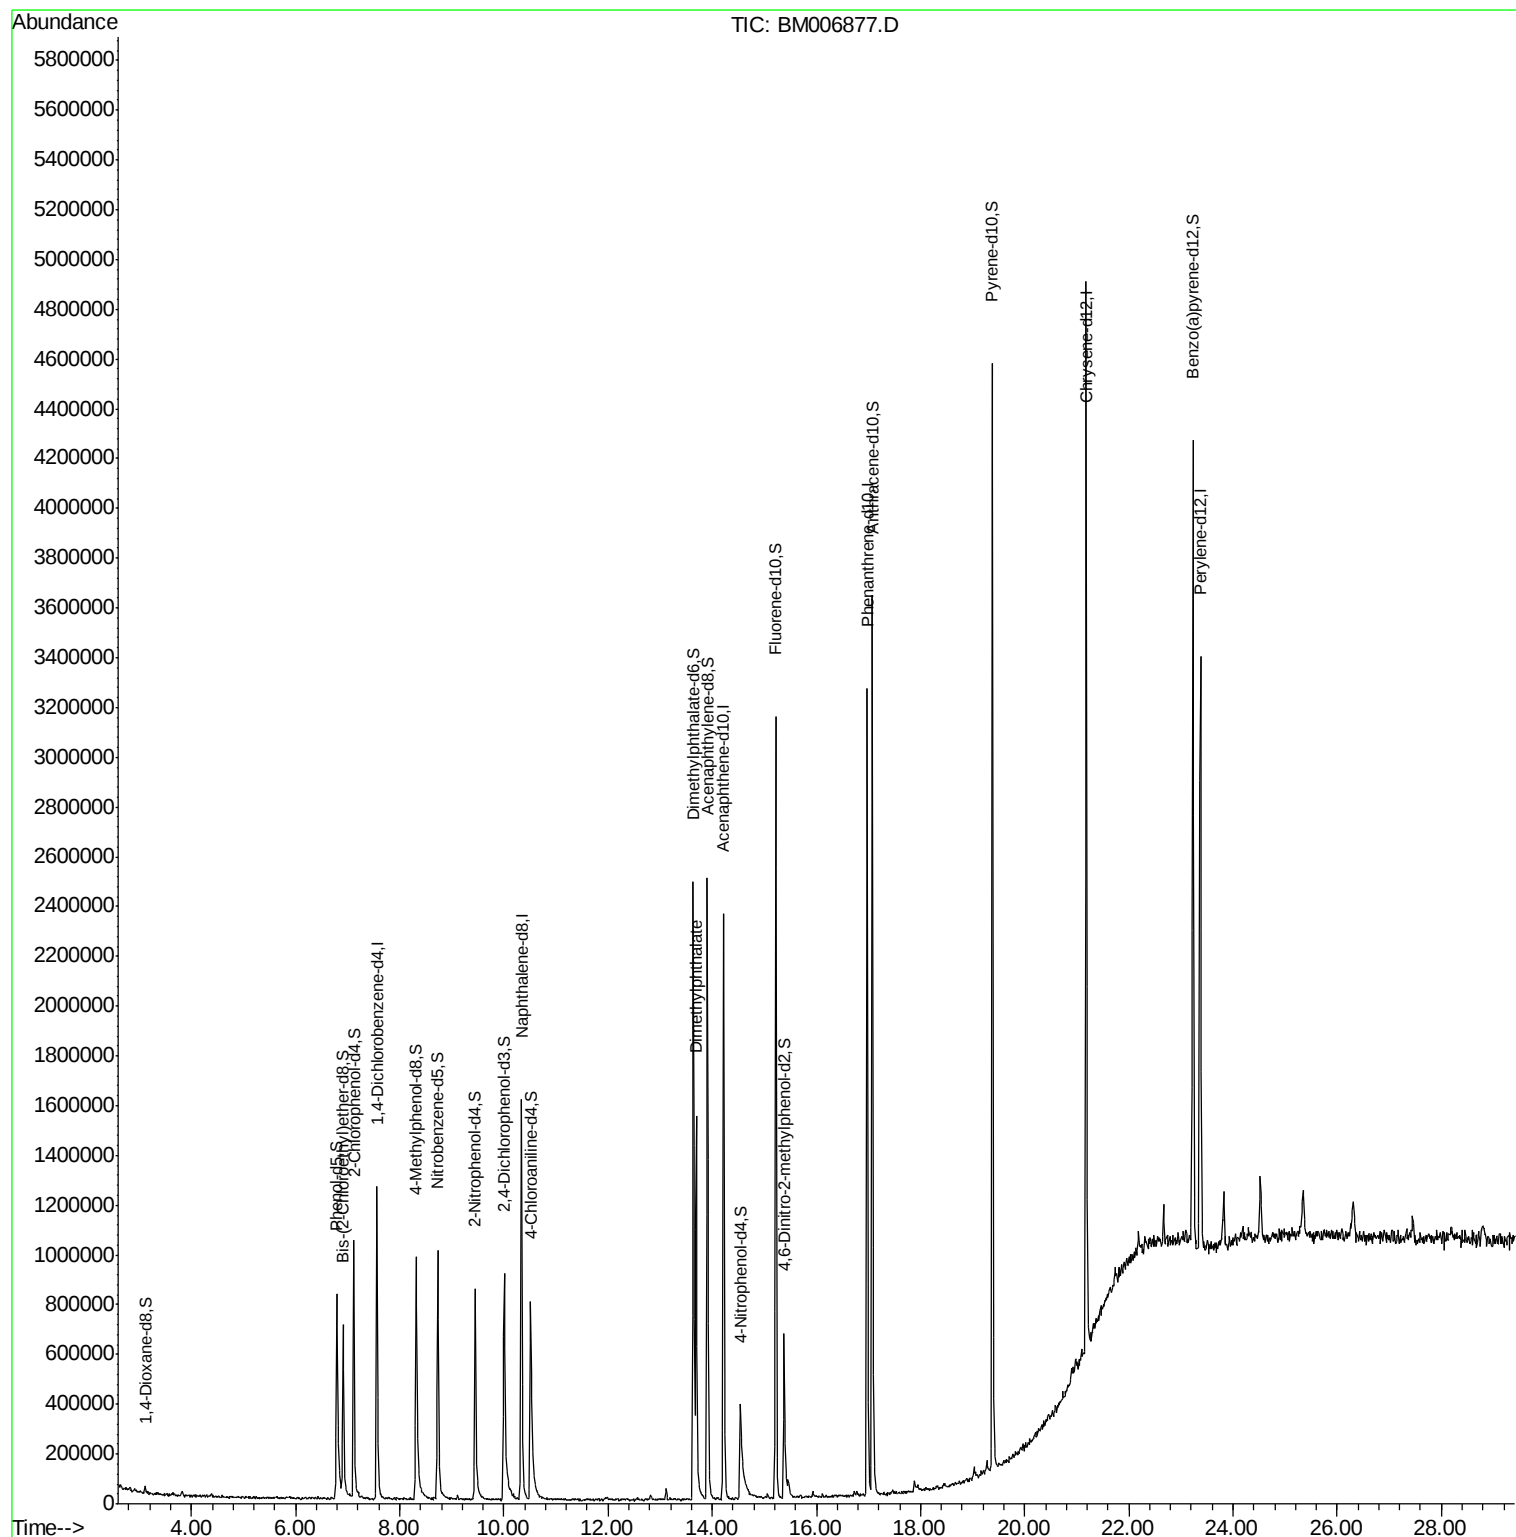

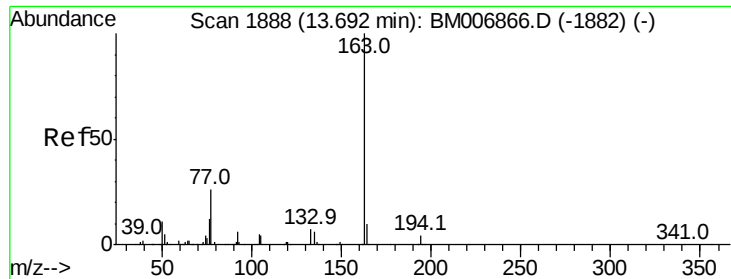

#44

Dimethylphthalate

Concen: 14.64 ng/ul

RT: 13.69 min Scan# 1888

Delta R.T. -0.01 min

Lab File: BM006877.D

Acq: 04 Aug 2016 23:21

Instrument :

BNA_M


ClientSampleId :

BDJH3

Tot Ion:	163	Resp:	892656
Ion Ratio	Lower	Upper	
163	100		
194	3.9	3.1	4.7
164	9.5	8.6	12.8

Manual Integrations
APPROVED

umangi
8/5/2016 7:01:20 PM

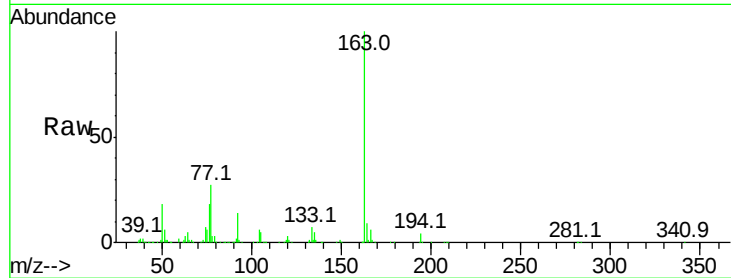

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

