

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080416\
 Data File : BM006864.D
 Acq On : 04 Aug 2016 15:28
 Operator : UM/SJ
 Sample : H4095-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJF9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.763	26	30	34	rBV4	57661	91011	2.06%	0.173%
2	6.798	710	716	731	rBV	528720	1293410	29.24%	2.461%
3	6.916	731	736	748	rVB	456157	769842	17.40%	1.465%
4	7.122	765	771	785	rBV	680330	1319932	29.84%	2.511%
5	7.563	839	846	862	rBV	947406	1757662	39.74%	3.344%
6	8.322	968	975	990	rBV2	579779	1428199	32.29%	2.717%
7	8.734	1037	1045	1064	rBV	671567	1372798	31.04%	2.612%
8	9.451	1159	1167	1188	rBV	532331	1231236	27.84%	2.342%
9	10.010	1254	1262	1281	rBV2	575539	1592069	35.99%	3.029%
10	10.339	1310	1318	1331	rBV	1186105	2270412	51.33%	4.319%
11	10.522	1342	1349	1362	rBV2	469770	1293698	29.25%	2.461%
12	13.121	1786	1791	1800	rVB2	38996	68559	1.55%	0.130%
13	13.645	1873	1880	1885	rBV	1495577	2306885	52.15%	4.389%
14	13.692	1885	1888	1906	rVB	891011	1628393	36.81%	3.098%
15	13.916	1919	1926	1939	rBV	1578712	2579028	58.31%	4.907%
16	14.221	1972	1978	1994	rVB2	1715515	2852149	64.48%	5.426%
17	14.563	2029	2036	2052	rBV4	160415	610687	13.81%	1.162%
18	15.227	2142	2149	2162	rBV	2051480	3321419	75.09%	6.319%
19	15.386	2170	2176	2186	rBV4	302107	643567	14.55%	1.224%
20	15.463	2186	2189	2196	rVB9	43037	88826	2.01%	0.169%
21	15.933	2262	2269	2273	rBV7	26145	44367	1.00%	0.084%
22	16.980	2440	2447	2458	rBV	2331538	3620695	81.85%	6.888%
23	17.080	2458	2464	2477	rVV	2258152	3582189	80.98%	6.815%
24	17.886	2596	2601	2610	rBV9	72288	173233	3.92%	0.330%
25	19.180	2817	2821	2825	rBV7	38089	64990	1.47%	0.124%
26	19.280	2833	2838	2841	rBV5	50943	100462	2.27%	0.191%
27	19.386	2850	2856	2867	rBV	2853787	4423319	100.00%	8.415%
28	21.192	3158	3163	3172	rBV	2993335	4292922	97.05%	8.167%
29	23.238	3505	3511	3519	rVB2	2137267	4013196	90.73%	7.635%
30	23.380	3529	3535	3545	rVB	1825153	3726841	84.25%	7.090%


Sum of corrected areas: 52561996

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080416\
Data File : BM006864.D
Acq On : 04 Aug 2016 15:28
Operator : UM/SJ
Sample : H4095-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJF9

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

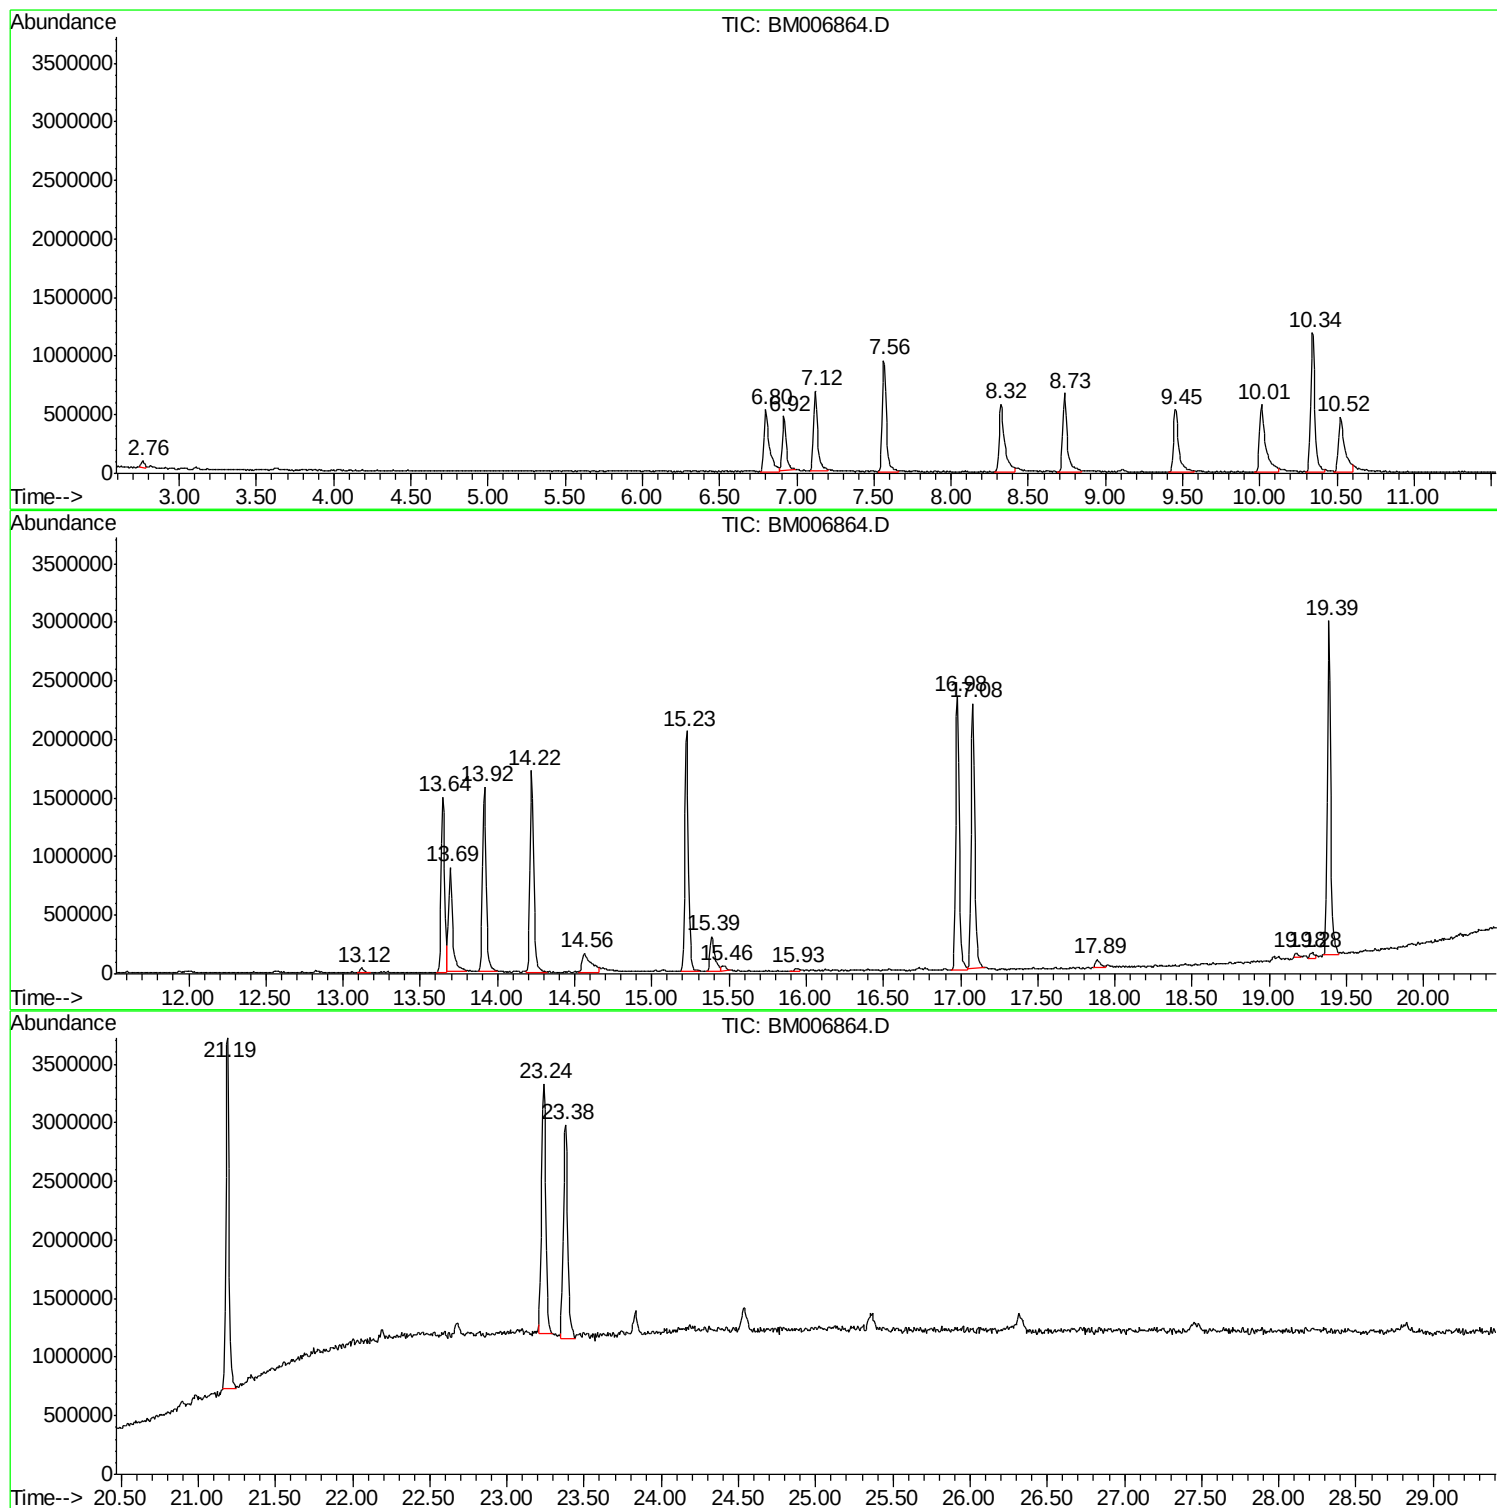

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080416\
Data File : BM006864.D
Acq On : 04 Aug 2016 15:28
Operator : UM/SJ
Sample : H4095-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJF9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080416\
Data File : BM006864.D
Acq On : 04 Aug 2016 15:28
Operator : UM/SJ
Sample : H4095-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJF9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc