

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080416\
 Data File : BM006879.D
 Acq On : 05 Aug 2016 00:33
 Operator : UM/SJ
 Sample : H4095-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJH6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.793	709	715	730	rBV2	689695	1618286	29.63%	2.482%
2	6.916	730	736	747	rVB	551209	978022	17.91%	1.500%
3	7.116	764	770	790	rBV	843502	1639454	30.02%	2.515%
4	7.563	840	846	860	rBV	1263320	2277351	41.70%	3.493%
5	8.316	967	974	993	rBV2	750373	1838865	33.67%	2.821%
6	8.734	1038	1045	1059	rBV	769998	1618790	29.64%	2.483%
7	9.451	1158	1167	1182	rBV	676573	1471549	26.95%	2.257%
8	10.004	1255	1261	1288	rBV	726692	2028017	37.13%	3.111%
9	10.339	1311	1318	1332	rBV	1630205	2972714	54.43%	4.560%
10	10.516	1341	1348	1368	rBV	648342	1781135	32.61%	2.732%
11	13.639	1869	1879	1884	rBV	1955937	2860050	52.37%	4.387%
12	13.686	1884	1887	1905	rVB	1154564	2105672	38.56%	3.230%
13	13.910	1918	1925	1942	rVB	1884590	3127324	57.26%	4.797%
14	14.216	1971	1977	1989	rBV2	2270567	3800326	69.59%	5.829%
15	14.551	2029	2034	2052	rBV3	216921	807359	14.78%	1.238%
16	15.221	2139	2148	2161	rBV	2514563	4001992	73.28%	6.138%
17	15.386	2170	2176	2186	rBV	376991	822678	15.06%	1.262%
18	15.468	2186	2190	2194	rVB6	53708	91206	1.67%	0.140%
19	15.933	2265	2269	2276	rBV4	33295	74612	1.37%	0.114%
20	16.727	2397	2404	2409	rBV6	34323	64878	1.19%	0.100%
21	16.974	2440	2446	2457	rBV2	3145269	4723092	86.48%	7.244%
22	17.074	2457	2463	2477	rVB	2575348	4294973	78.64%	6.588%
23	17.886	2595	2601	2608	rBV	52436	126740	2.32%	0.194%
24	19.027	2791	2795	2799	rBV4	38061	75342	1.38%	0.116%
25	19.380	2847	2855	2865	rBV	3431459	5239983	95.95%	8.037%
26	21.186	3157	3162	3169	rBV	4004460	5461226	100.00%	8.377%
27	23.233	3504	3510	3521	rVB	2426258	4775598	87.45%	7.325%
28	23.374	3528	3534	3543	rVB	2423184	4518961	82.75%	6.931%


Sum of corrected areas: 65196195

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080416\
Data File : BM006879.D
Acq On : 05 Aug 2016 00:33
Operator : UM/SJ
Sample : H4095-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJH6

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

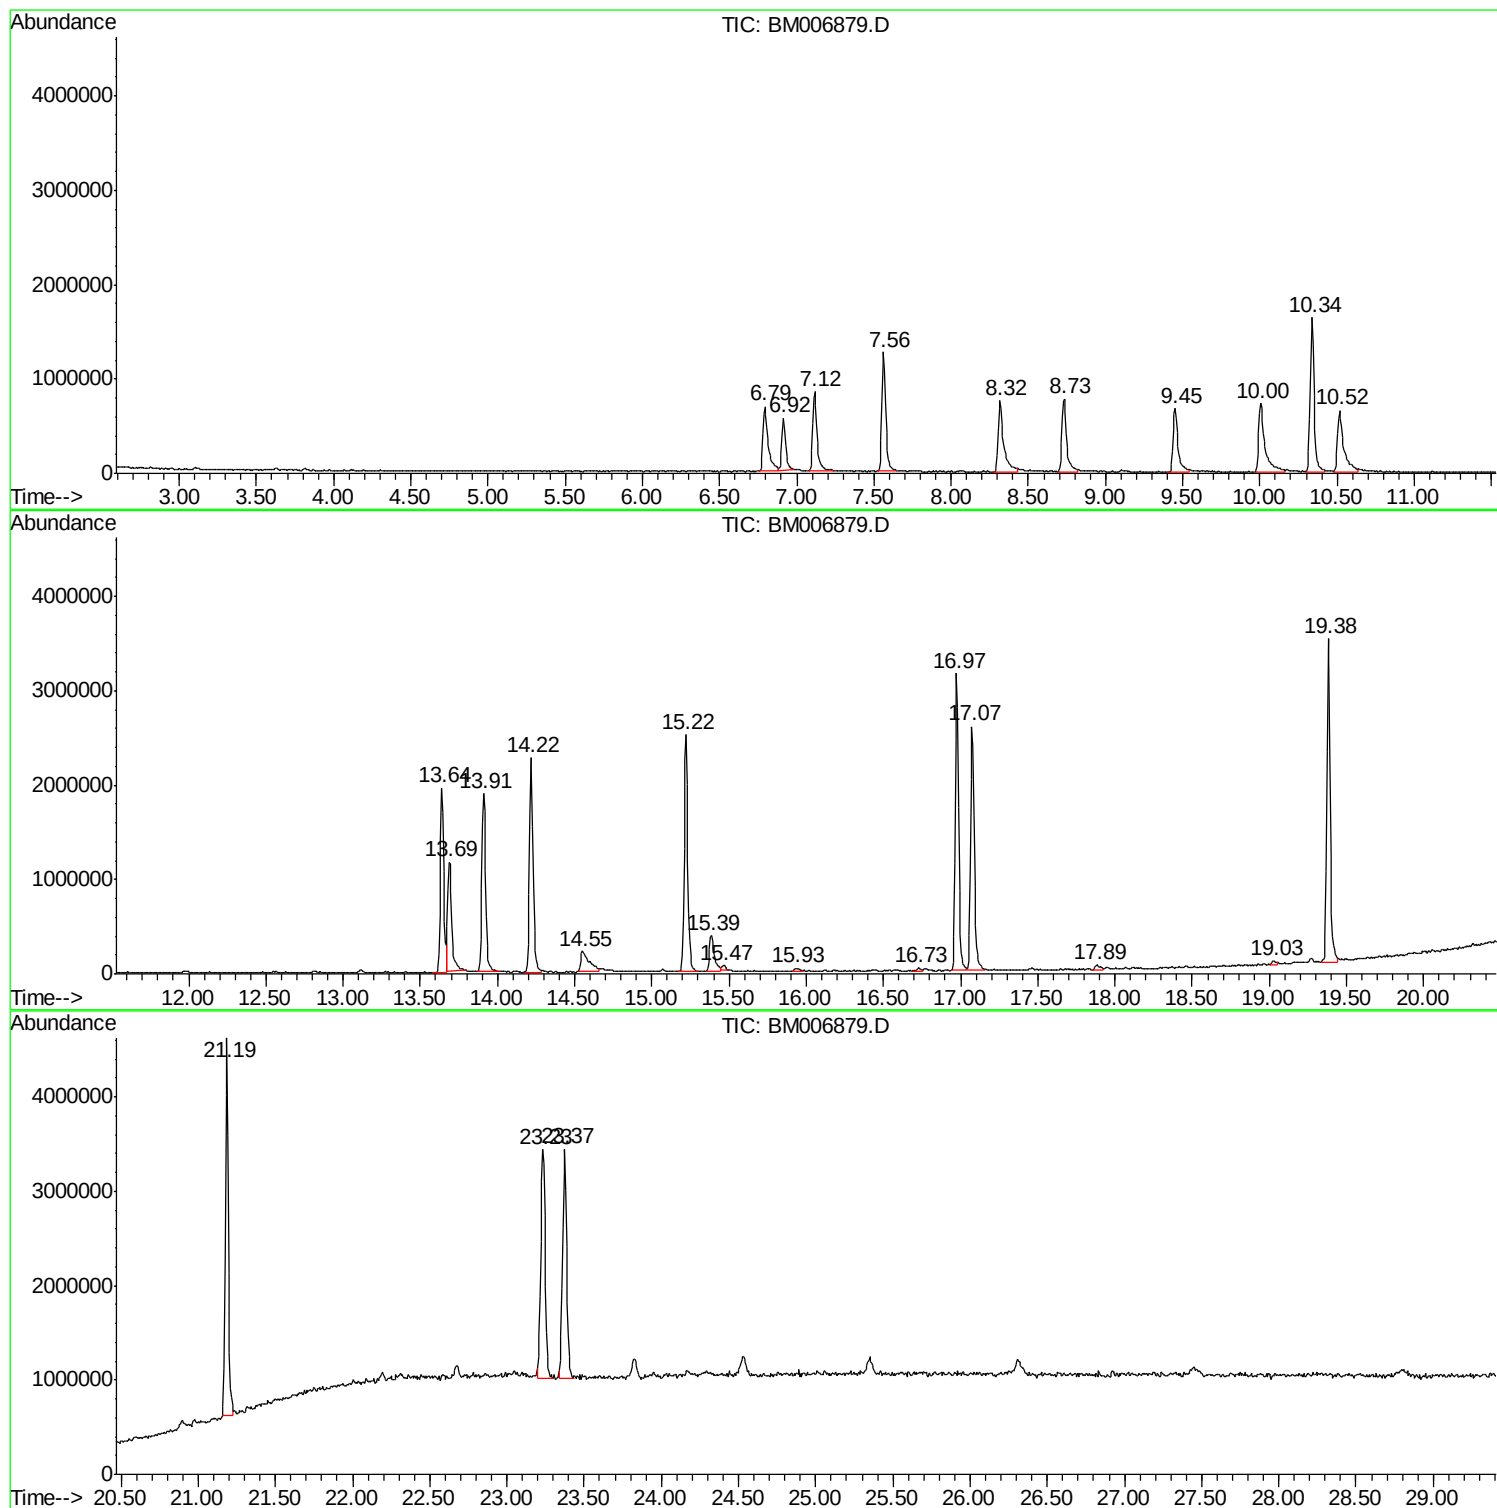

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080416\
Data File : BM006879.D
Acq On : 05 Aug 2016 00:33
Operator : UM/SJ
Sample : H4095-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJH6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080416\
Data File : BM006879.D
Acq On : 05 Aug 2016 00:33
Operator : UM/SJ
Sample : H4095-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJH6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc