

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080416\
 Data File : BM006887.D
 Acq On : 05 Aug 2016 05:26
 Operator : UM/SJ
 Sample : H4224-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJL6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.792	707	715	731	rBV	505087	1271104	22.08%	2.139%
2	6.916	731	736	751	rVB	476521	865203	15.03%	1.456%
3	7.116	764	770	781	rBV	681919	1262694	21.94%	2.125%
4	7.563	840	846	862	rVB	1208355	2171933	37.74%	3.655%
5	8.316	967	974	995	rBV	563980	1498373	26.03%	2.522%
6	8.733	1037	1045	1060	rBV	645493	1376933	23.92%	2.317%
7	9.451	1161	1167	1183	rBV2	528112	1182728	20.55%	1.990%
8	10.004	1255	1261	1281	rBV2	533626	1547104	26.88%	2.604%
9	10.339	1307	1318	1331	rBV	1619193	3026195	52.58%	5.093%
10	10.522	1342	1349	1376	rBV2	466179	1468268	25.51%	2.471%
11	13.639	1869	1879	1884	rBV	1522124	2360453	41.01%	3.972%
12	13.692	1884	1888	1902	rVB	563882	1103839	19.18%	1.858%
13	13.910	1918	1925	1938	rBV	1625141	2635748	45.79%	4.436%
14	14.215	1970	1977	1992	rBV2	2410218	3940669	68.47%	6.631%
15	14.551	2029	2034	2055	rBV3	210819	937362	16.29%	1.577%
16	15.221	2138	2148	2164	rBV	2129166	3543926	61.57%	5.964%
17	15.386	2170	2176	2186	rBV2	393192	885822	15.39%	1.491%
18	15.462	2186	2189	2199	rVB9	47102	103471	1.80%	0.174%
19	16.727	2400	2404	2408	rBV4	43094	58452	1.02%	0.098%
20	16.768	2408	2411	2422	rVB8	34806	66070	1.15%	0.111%
21	16.974	2439	2446	2457	rBV	3182845	4931833	85.69%	8.299%
22	17.074	2457	2463	2474	rVV2	2358459	3795964	65.95%	6.388%
23	17.880	2594	2600	2603	rBV7	68645	103720	1.80%	0.175%
24	17.951	2608	2612	2617	rVB4	36067	64954	1.13%	0.109%
25	19.056	2796	2800	2804	rVB2	65374	95406	1.66%	0.161%
26	19.380	2850	2855	2866	rBV	2876899	4570206	79.40%	7.691%
27	21.186	3156	3162	3171	rBV	4035581	5755584	100.00%	9.686%
28	23.233	3504	3510	3517	rVB2	2115899	3897932	67.72%	6.560%
29	23.368	3527	3533	3547	rVB2	2507780	4901847	85.17%	8.249%


Sum of corrected areas: 59423793

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080416\
Data File : BM006887.D
Acq On : 05 Aug 2016 05:26
Operator : UM/SJ
Sample : H4224-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJL6

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

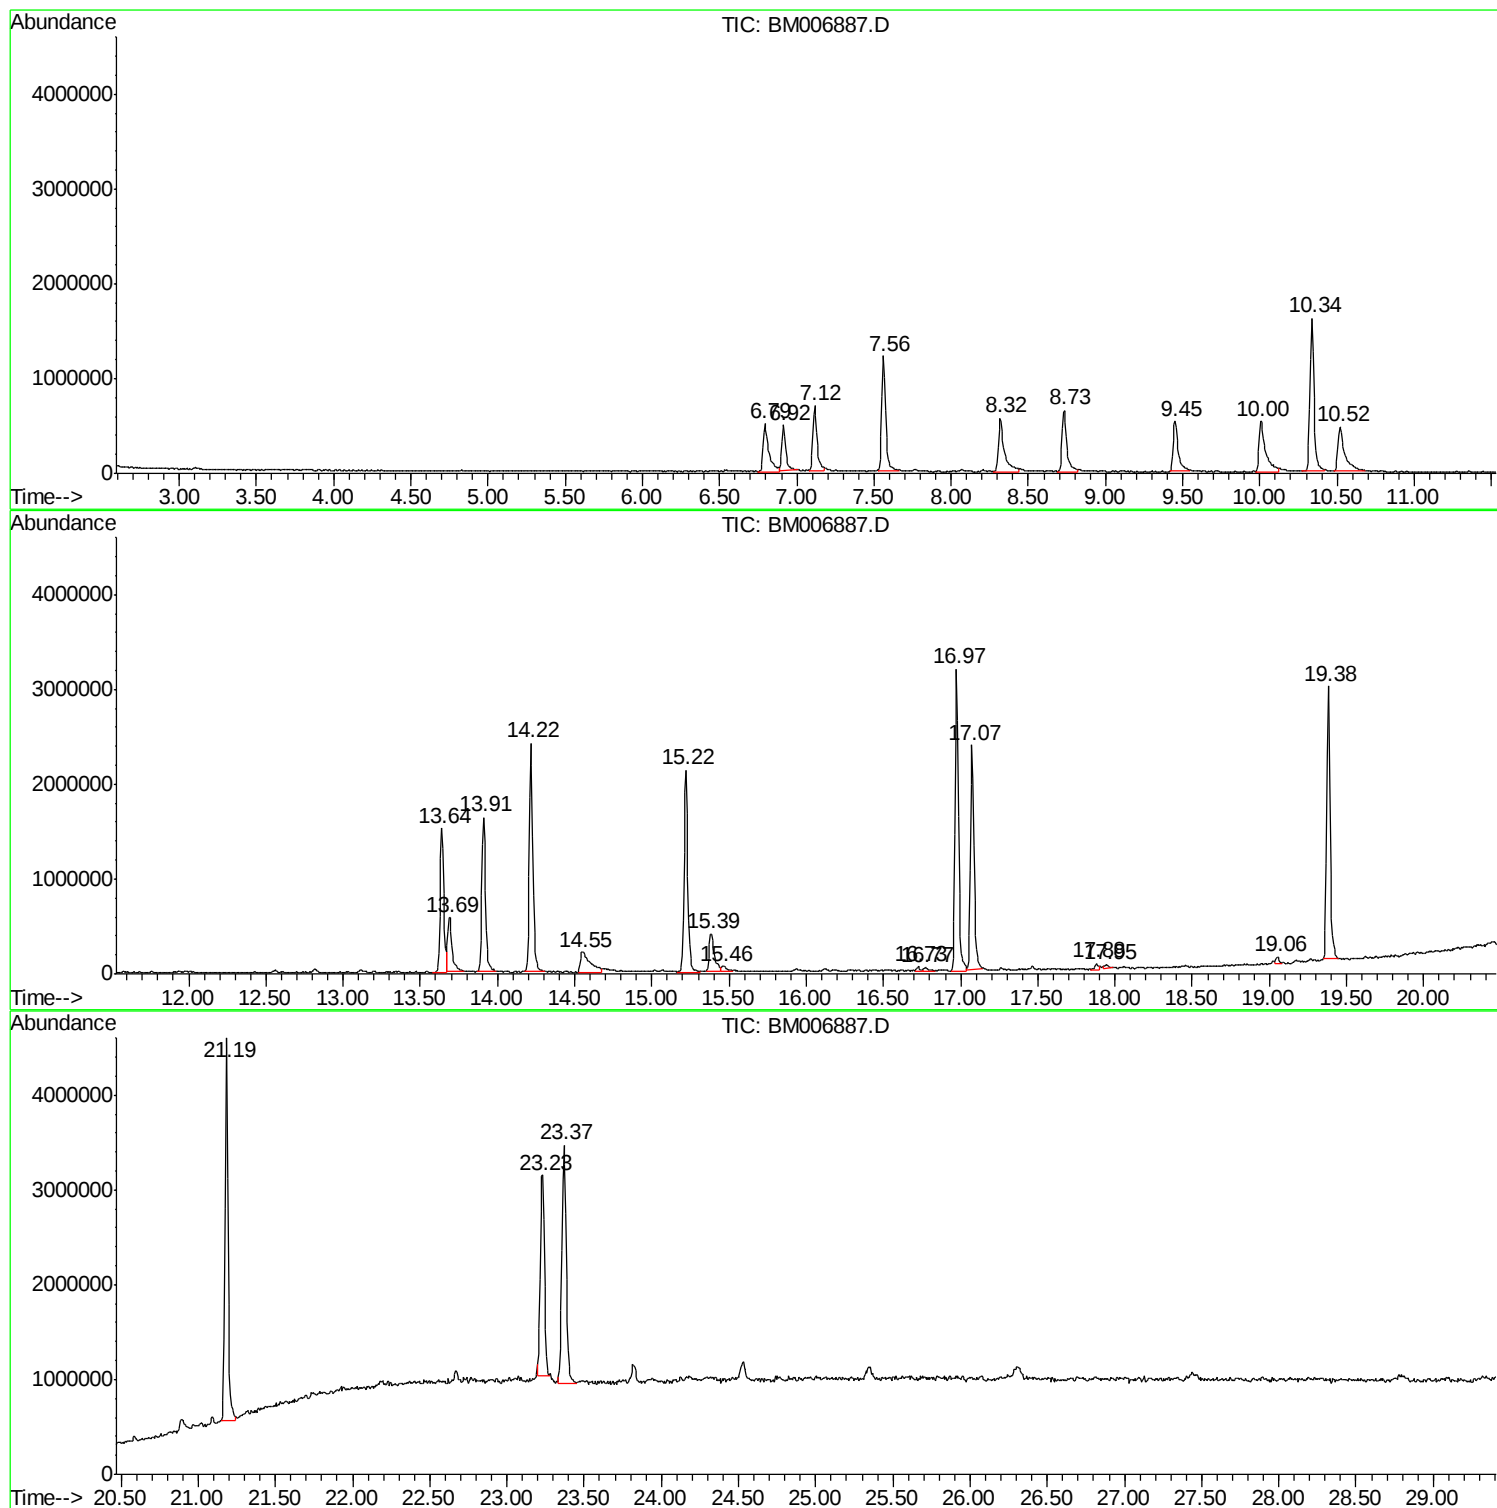

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080416\
Data File : BM006887.D
Acq On : 05 Aug 2016 05:26
Operator : UM/SJ
Sample : H4224-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJL6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080416\
Data File : BM006887.D
Acq On : 05 Aug 2016 05:26
Operator : UM/SJ
Sample : H4224-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJL6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc