
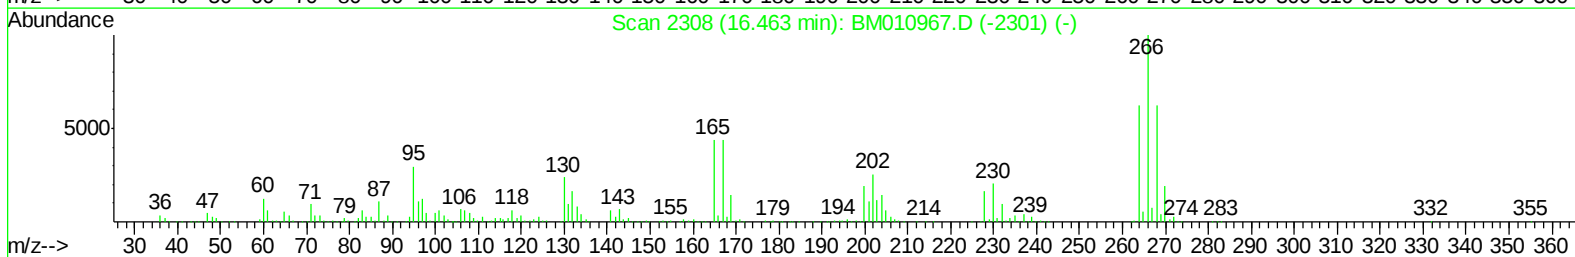
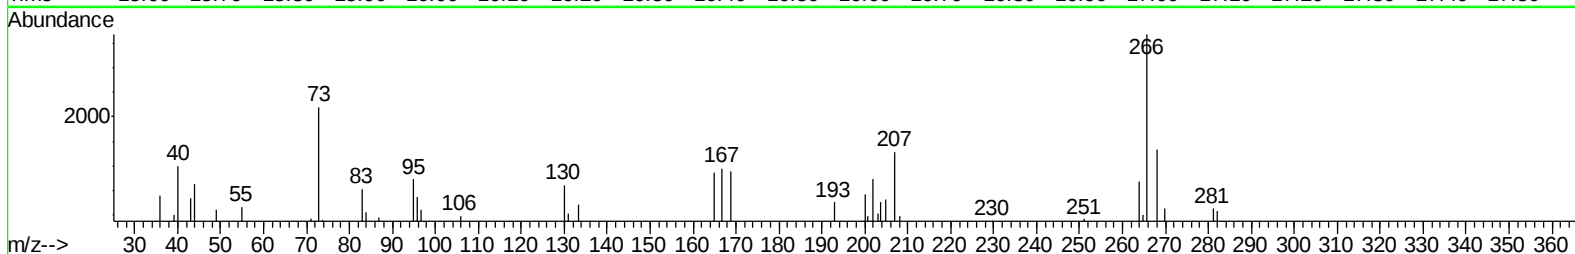


Data Path : Z:\HPCHEM1\BNA_M\Data\BM080417\
Data File : BM011118.D
Acq On : 04 Aug 2017 13:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 18:29:31 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

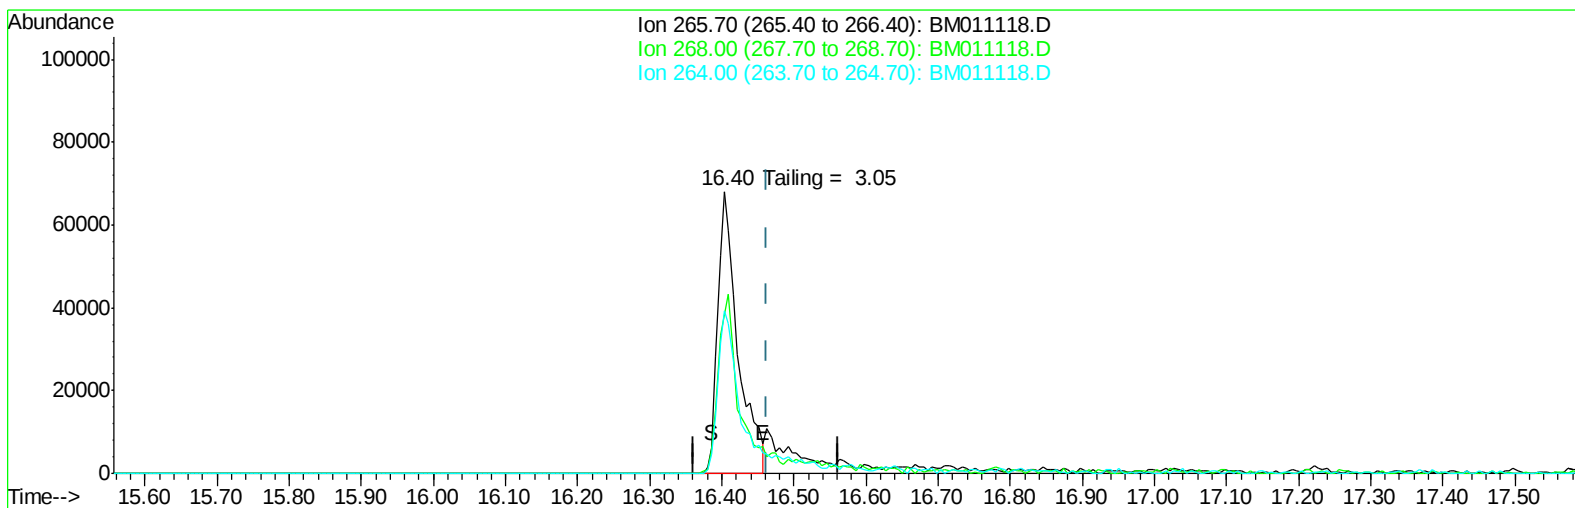

TIC: BM011118.D

(69) Pentachlorophenol (C)




16.563min (+0.100) 1219.39ng

response 2058

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	43.98#
264.00	61.20	40.21#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM080417\
Data File : BM011118.D
Acq On : 04 Aug 2017 13:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 18:29:31 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

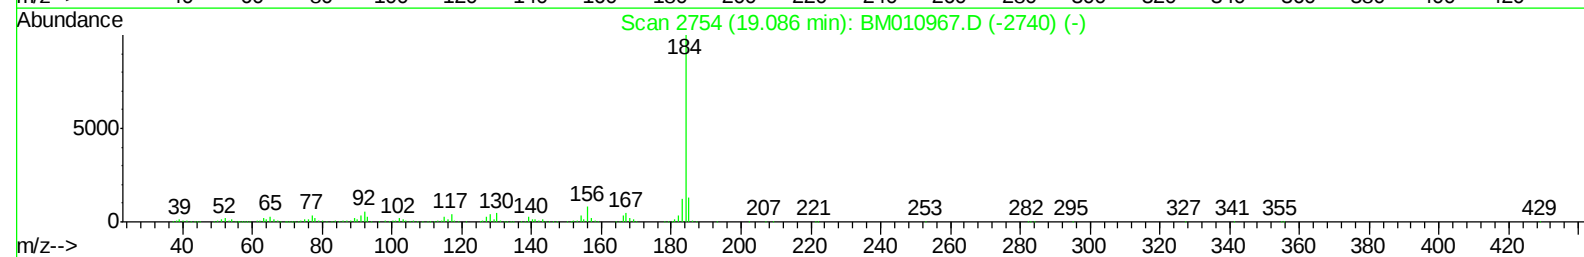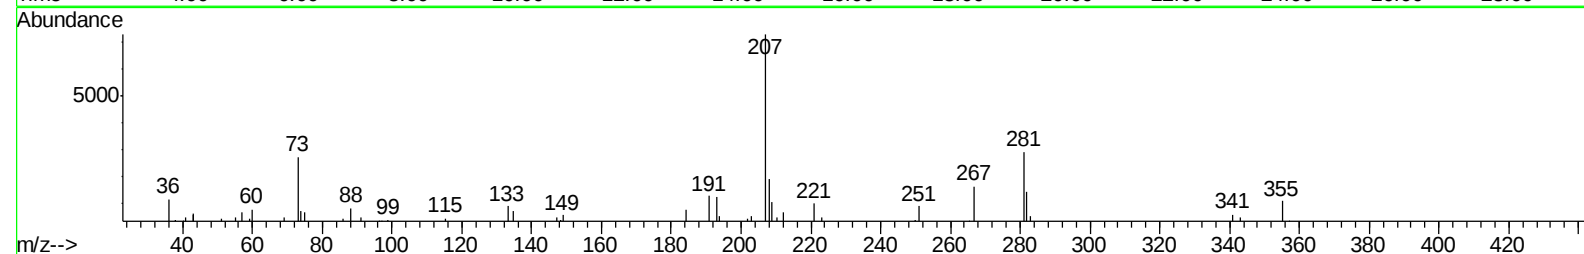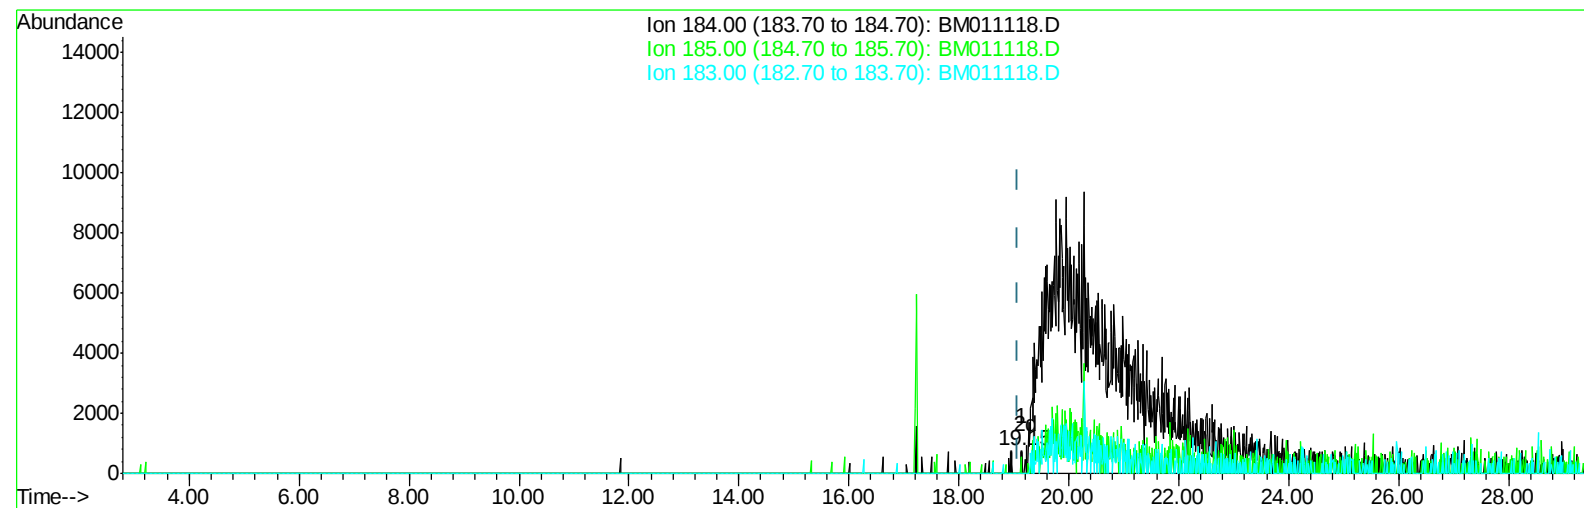

TIC: BM011118.D

(76) Benzidine

19.151min (+0.065) 5.50ng

response 259

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	0.00#
183.00	11.10	0.00#
0.00	0.00	0.00