


Data Path : Z:\HPCHEM1\BNA M\Data\BM080417\
 Data File : BM011118.D
 Acq On : 04 Aug 2017 13:44
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

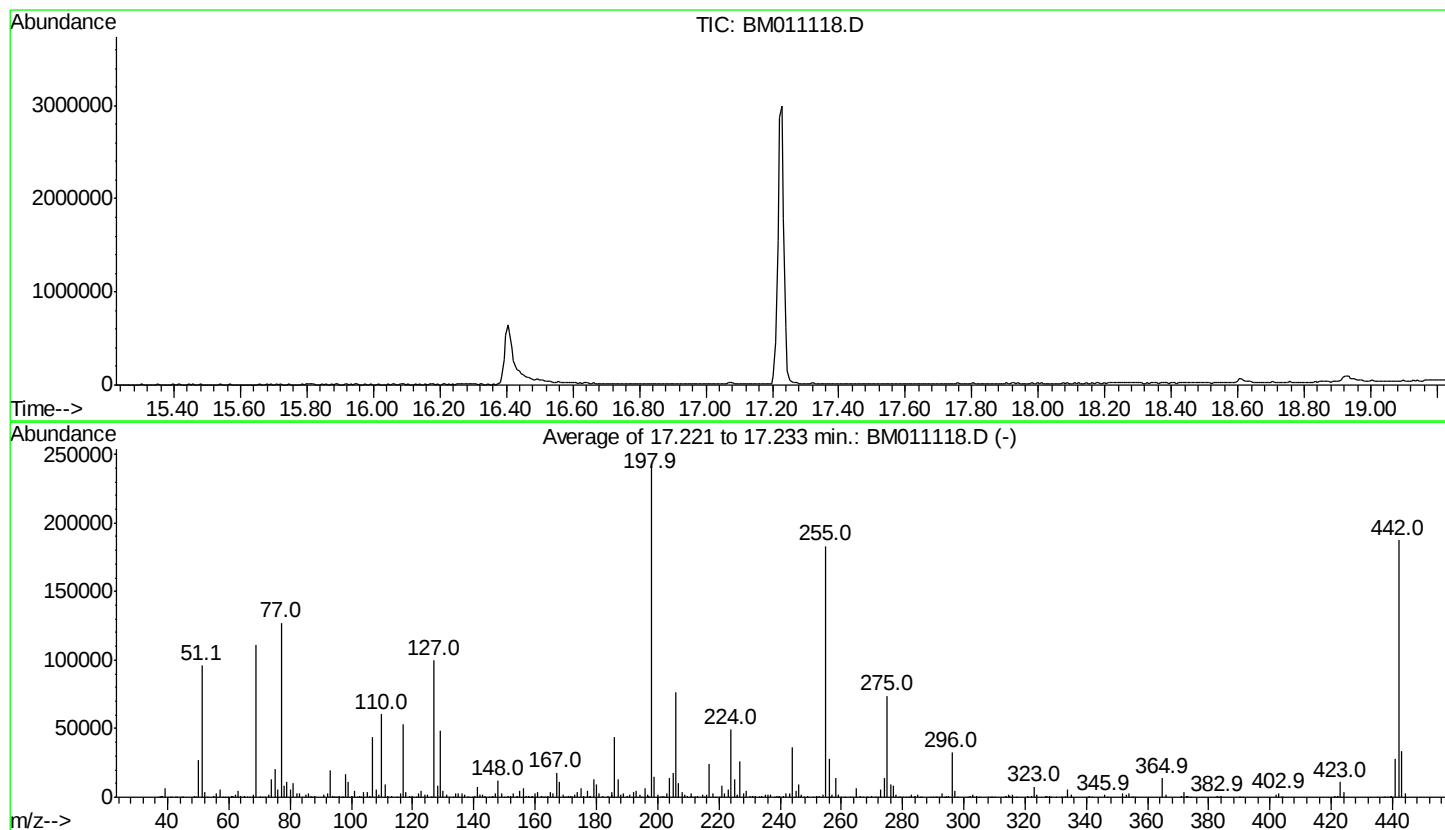

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	95872	PASS
68	69	0.00	2	1.6	1733	PASS
69	198	0.00	100	46.1	111498	PASS
70	69	0.00	2	0.3	304	PASS
127	198	10	80	41.2	99573	PASS
197	198	0.00	2	0.9	2168	PASS
198	198	100	100	100.0	241706	PASS
199	198	5	9	6.3	15257	PASS
275	198	10	60	30.5	73760	PASS
365	198	1	100	5.8	13979	PASS
441	443	0.01	100	83.2	28072	PASS
442	198	50	100	77.6	187541	PASS
443	442	15	24	18.0	33744	PASS