

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080422\
 Data File : BM036094.D
 Acq On : 04 Aug 2022 12:11
 Operator : CG/JU
 Sample : PB146679BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146679BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	390	397	410	rBV	5442804	7635689	55.98%	11.053%
2	7.034	663	671	684	rBV	4997375	7722154	56.61%	11.179%
3	7.857	803	811	822	rBV	1033425	1592583	11.68%	2.305%
4	9.028	1001	1010	1027	rBV	3092266	4965365	36.40%	7.188%
5	10.663	1280	1288	1303	rBV	1394250	2302930	16.88%	3.334%
6	13.128	1700	1707	1720	rBV	8127628	11366264	83.33%	16.454%
7	14.498	1933	1940	1954	rBV	2068614	2910381	21.34%	4.213%
8	15.986	2186	2193	2204	rBV	5850423	8188412	60.03%	11.854%
9	17.239	2400	2406	2416	rBV	2308090	3167099	23.22%	4.585%
10	19.868	2847	2853	2861	rBV	11641245	13640510	100.00%	19.746%
11	21.421	3112	3117	3123	rBV	2312534	2908641	21.32%	4.211%
12	23.786	3513	3519	3528	rVB2	1365601	2679918	19.65%	3.879%




Sum of corrected areas: 69079946

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080422\
Data File : BM036094.D
Acq On : 04 Aug 2022 12:11
Operator : CG/JU
Sample : PB146679BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146679BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

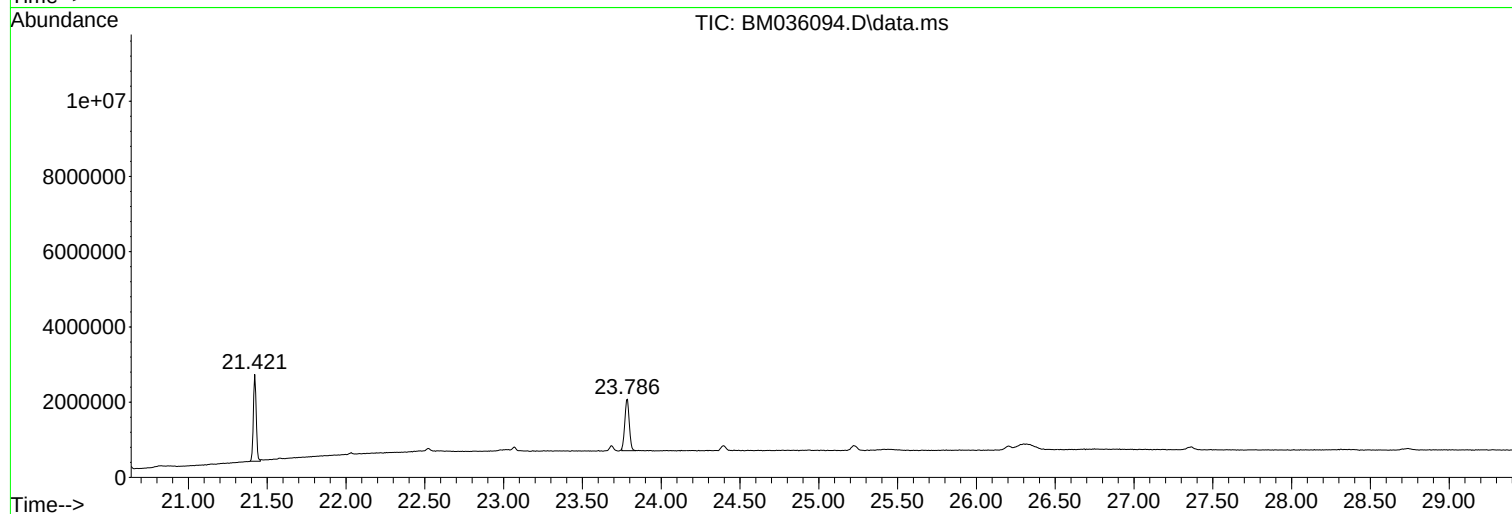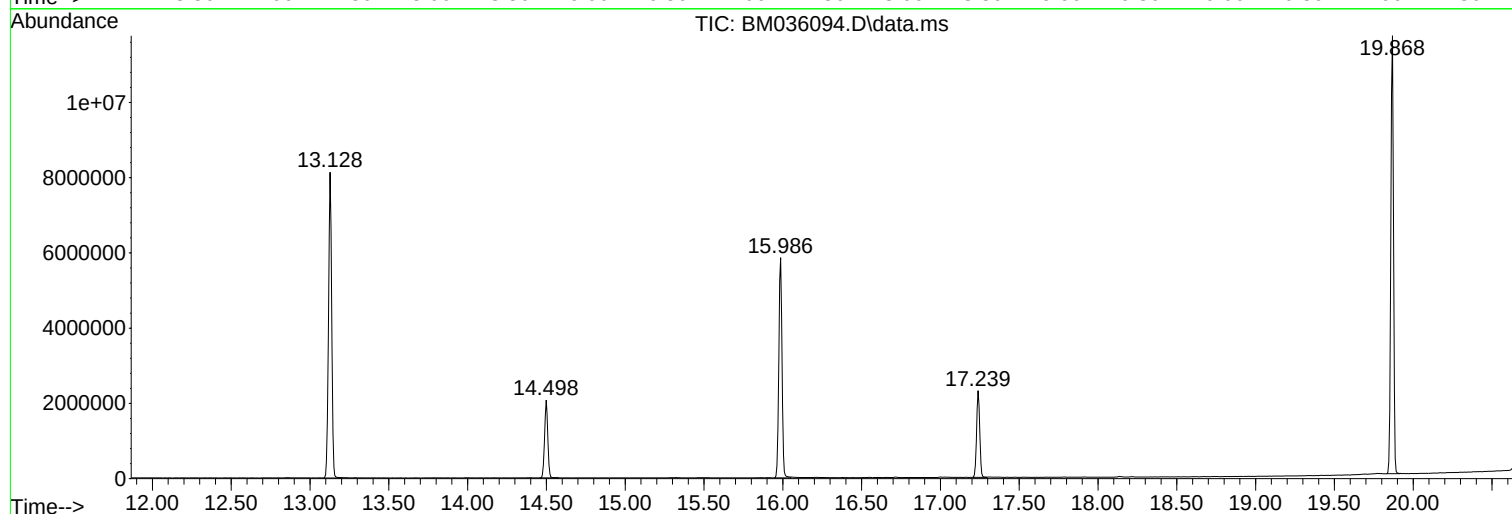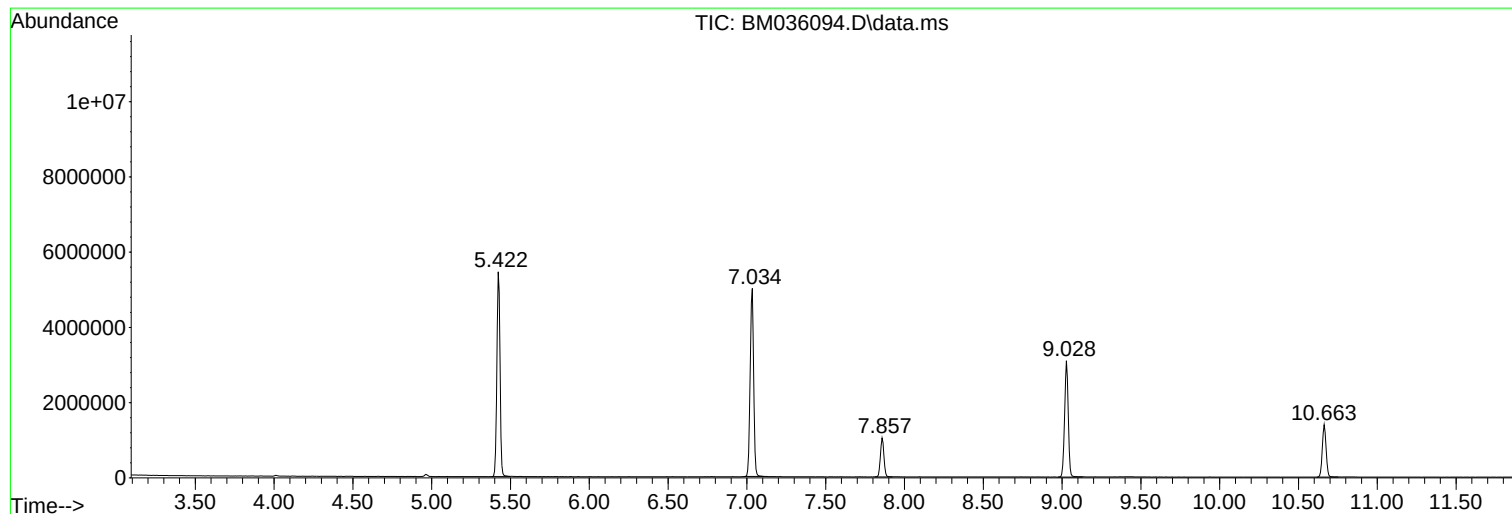

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080422\
Data File : BM036094.D
Acq On : 04 Aug 2022 12:11
Operator : CG/JU
Sample : PB146679BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146679BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080422\
Data File : BM036094.D
Acq On : 04 Aug 2022 12:11
Operator : CG/JU
Sample : PB146679BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146679BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------