

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080422\
 Data File : BM036105.D
 Acq On : 04 Aug 2022 19:07
 Operator : CG/JU
 Sample : N3931-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 RVE-116

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	391	398	414	rBV	5887306	8354406	39.78%	7.817%
2	7.040	660	672	685	rBV	5913466	9167973	43.65%	8.578%
3	7.857	800	811	819	rBV	1117783	1776262	8.46%	1.662%
4	9.028	1002	1010	1025	rBV	3494150	5888005	28.03%	5.509%
5	10.663	1280	1288	1295	rBV	1625938	2750153	13.09%	2.573%
6	13.127	1699	1707	1723	rBV	9649530	14195042	67.58%	13.281%
7	14.498	1931	1940	1947	rBV	2563117	3756850	17.89%	3.515%
8	15.986	2186	2193	2202	rBV	8121556	11809652	56.23%	11.049%
9	16.204	2224	2230	2239	rBV4	77503	210975	1.00%	0.197%
10	17.245	2397	2407	2411	rBV	3145433	4586603	21.84%	4.291%
11	17.286	2411	2414	2419	rVB	777419	994925	4.74%	0.931%
12	18.145	2556	2560	2562	rBV	279591	329729	1.57%	0.309%
13	18.304	2583	2587	2592	rBV3	135233	228577	1.09%	0.214%
14	19.033	2707	2711	2715	rBV	156439	235332	1.12%	0.220%
15	19.174	2731	2735	2741	rBV	159274	238107	1.13%	0.223%
16	19.298	2751	2756	2763	rBV	1802206	2278169	10.85%	2.132%
17	19.656	2813	2817	2826	rVB	1480645	2166202	10.31%	2.027%
18	19.868	2847	2853	2858	rBV	17144622	21003854	100.00%	19.652%
19	19.980	2868	2872	2880	rBV4	128368	328520	1.56%	0.307%
20	20.903	3025	3029	3035	rVB	289238	378865	1.80%	0.354%
21	21.139	3065	3069	3076	rVB2	2325451	2933286	13.97%	2.744%
22	21.421	3110	3117	3121	rBV2	3716410	5679121	27.04%	5.314%
23	21.456	3121	3123	3131	rVB	850190	1025488	4.88%	0.959%
24	21.580	3141	3144	3150	rBV2	242039	344947	1.64%	0.323%
25	22.033	3218	3221	3223	rBV	389167	485147	2.31%	0.454%
26	23.068	3392	3397	3402	rBV	763734	1522758	7.25%	1.425%
27	23.680	3498	3501	3509	rVB	513547	881424	4.20%	0.825%
28	23.786	3513	3519	3526	rBV2	1719017	3329791	15.85%	3.115%




Sum of corrected areas: 106880163

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080422\
Data File : BM036105.D
Acq On : 04 Aug 2022 19:07
Operator : CG/JU
Sample : N3931-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RVE-116

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

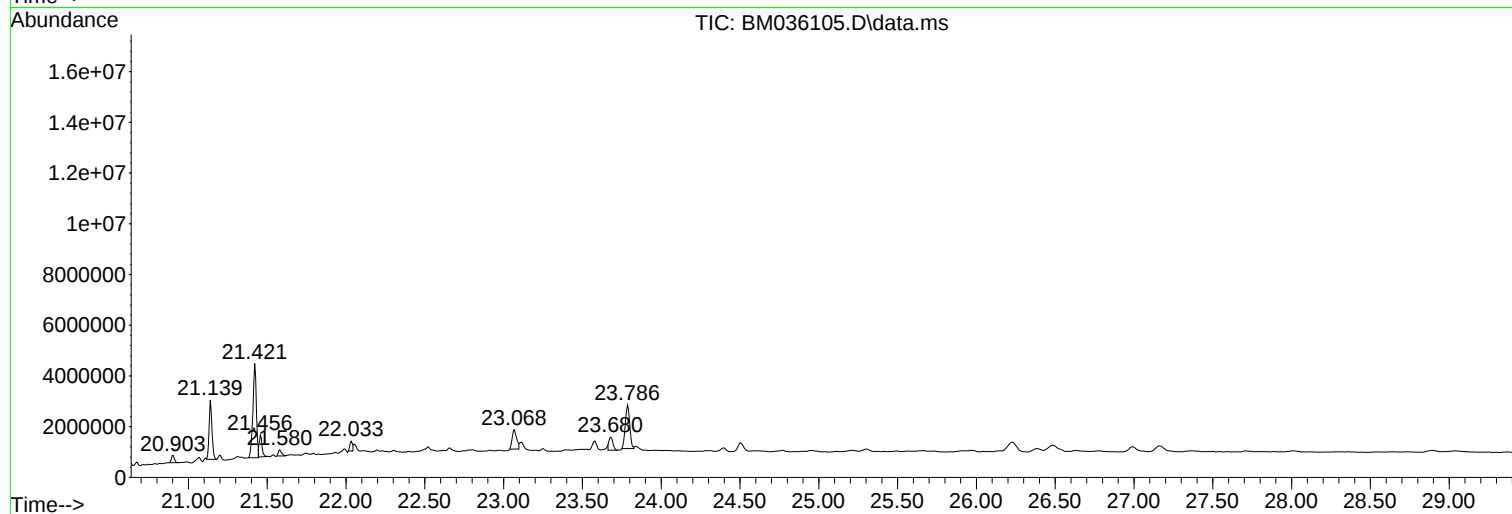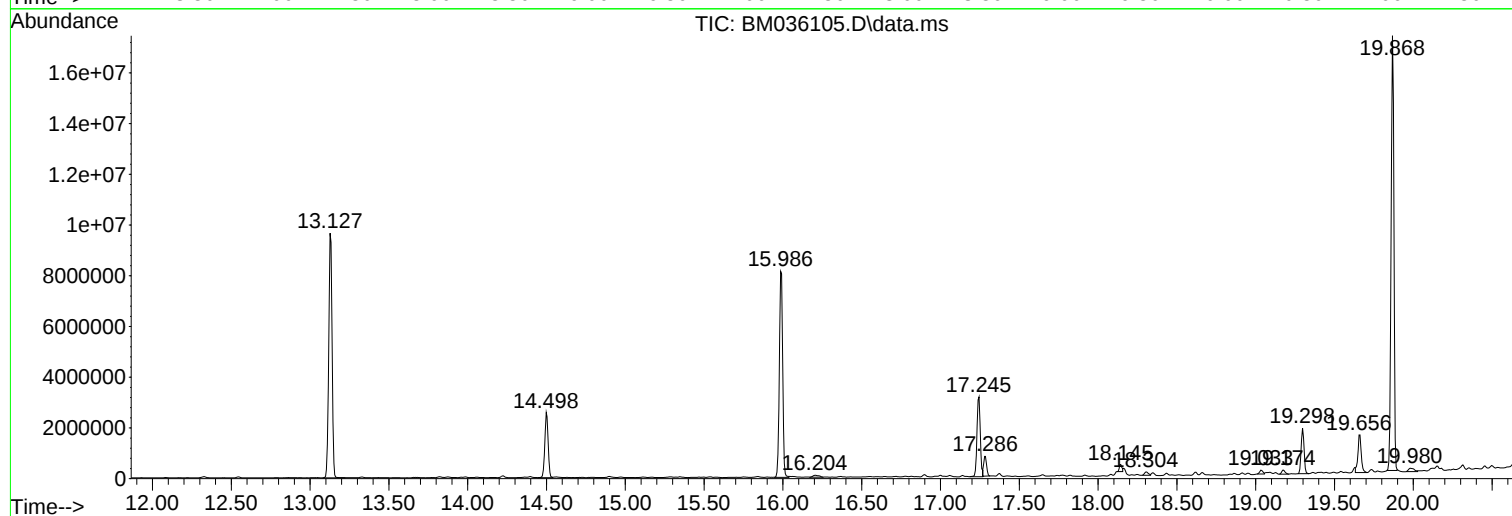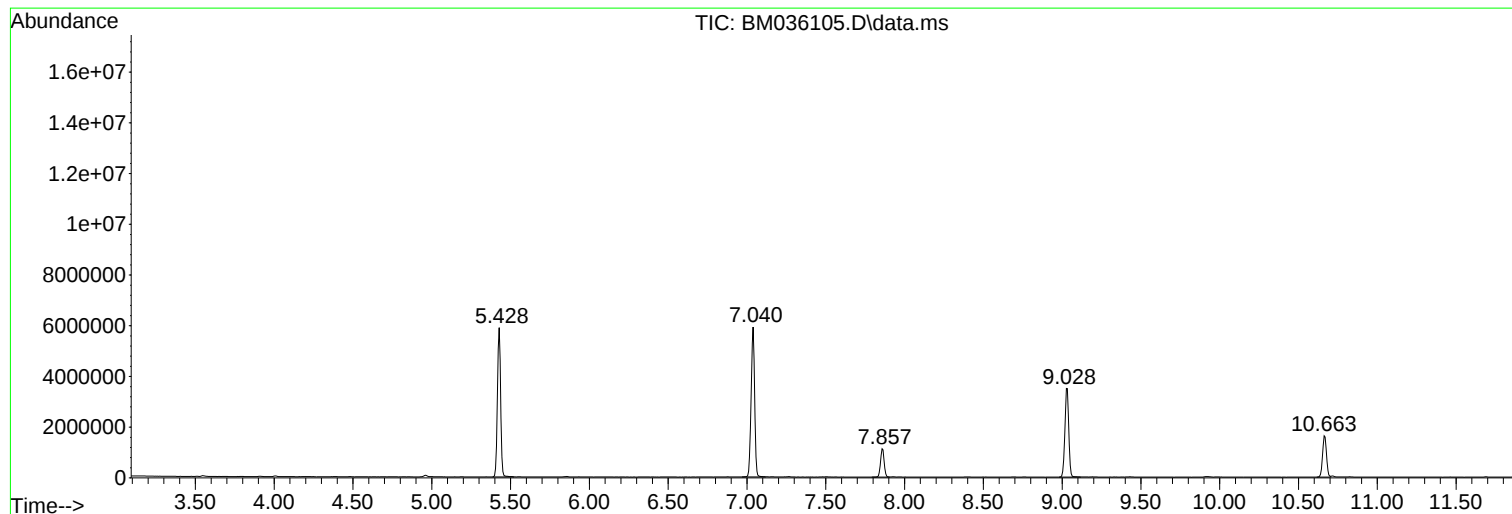

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080422\
Data File : BM036105.D
Acq On : 04 Aug 2022 19:07
Operator : CG/JU
Sample : N3931-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RVE-116










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(tetradecyloxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.139	10.33 ng	2933290	Chrysene-d12	21.421

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	96
2			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	95
3			Cyclohexadecane	224	C16H32	000295-65-8	94
4			Pentadecafluorooctanoic acid, he...	638	C24H33F15O2	1000406-04-6	94
5			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	93

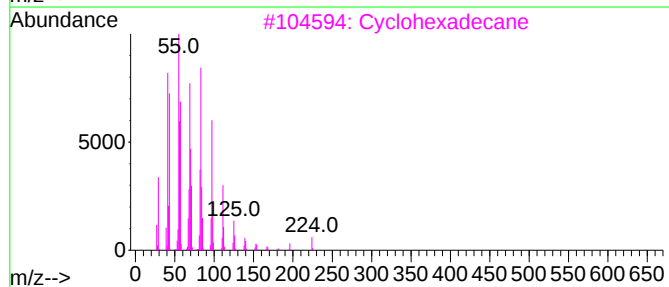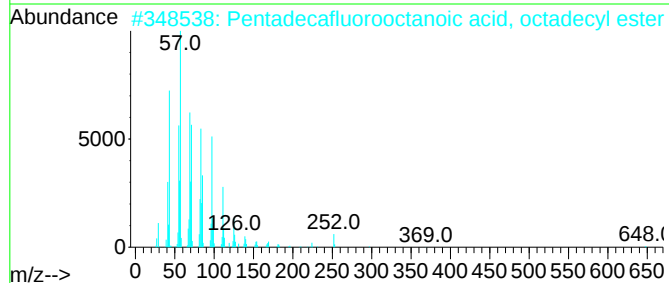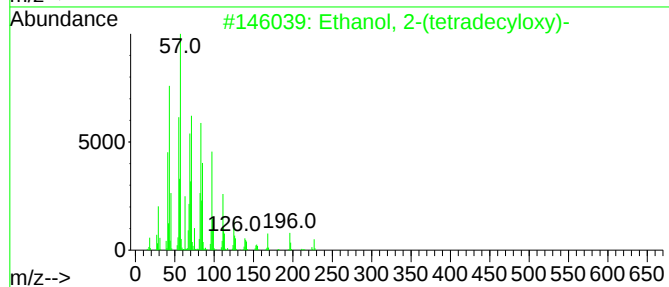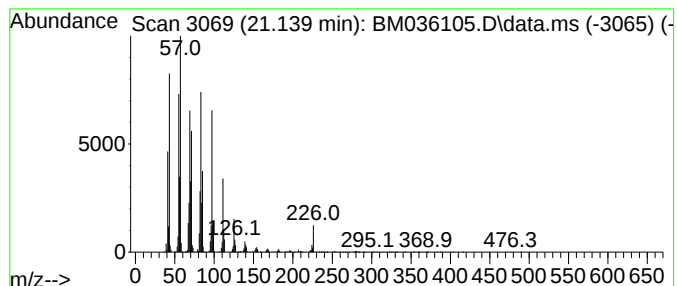

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080422\
Data File : BM036105.D
Acq On : 04 Aug 2022 19:07
Operator : CG/JU
Sample : N3931-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RVE-116

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(tet...	21.139	10.3	ng	2933290	5	21.421	5679120	20.0