

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006896.D
 Acq On : 05 Aug 2016 12:50
 Operator : UM/SJ
 Sample : H4224-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJN6

Quant Time: Aug 06 00:34:07 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 06 00:33:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	120407	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	503782	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	312909	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	731716	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	818788	20.00	ng/ul	0.00
83) Perylene-d12	23.37	264	782284	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	4314	1.97	ng/uL	0.00
5) Phenol-d5	6.79	99	194998	22.00	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	142866	24.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	158678	22.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	158578	22.00	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	77422	22.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	86501	21.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	140899	16.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	190411	21.74	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	583321	22.63	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	684591	21.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	11870	2.10	ng/ul	0.03
57) Fluorene-d10	15.22	176	503454	21.04	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	35131	7.36	ng/ul	0.01
70) Anthracene-d10	17.07	188	775868	22.08	ng/ul	0.00
76) Pyrene-d10	19.38	212	915320	21.85	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.23	264	848509	22.27	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.69	163	247374	9.66	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006896.D
Acq On : 05 Aug 2016 12:50
Operator : UM/SJ
Sample : H4224-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJN6

Quant Time: Aug 06 00:34:07 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 06 00:33:11 2016
Response via : Initial Calibration

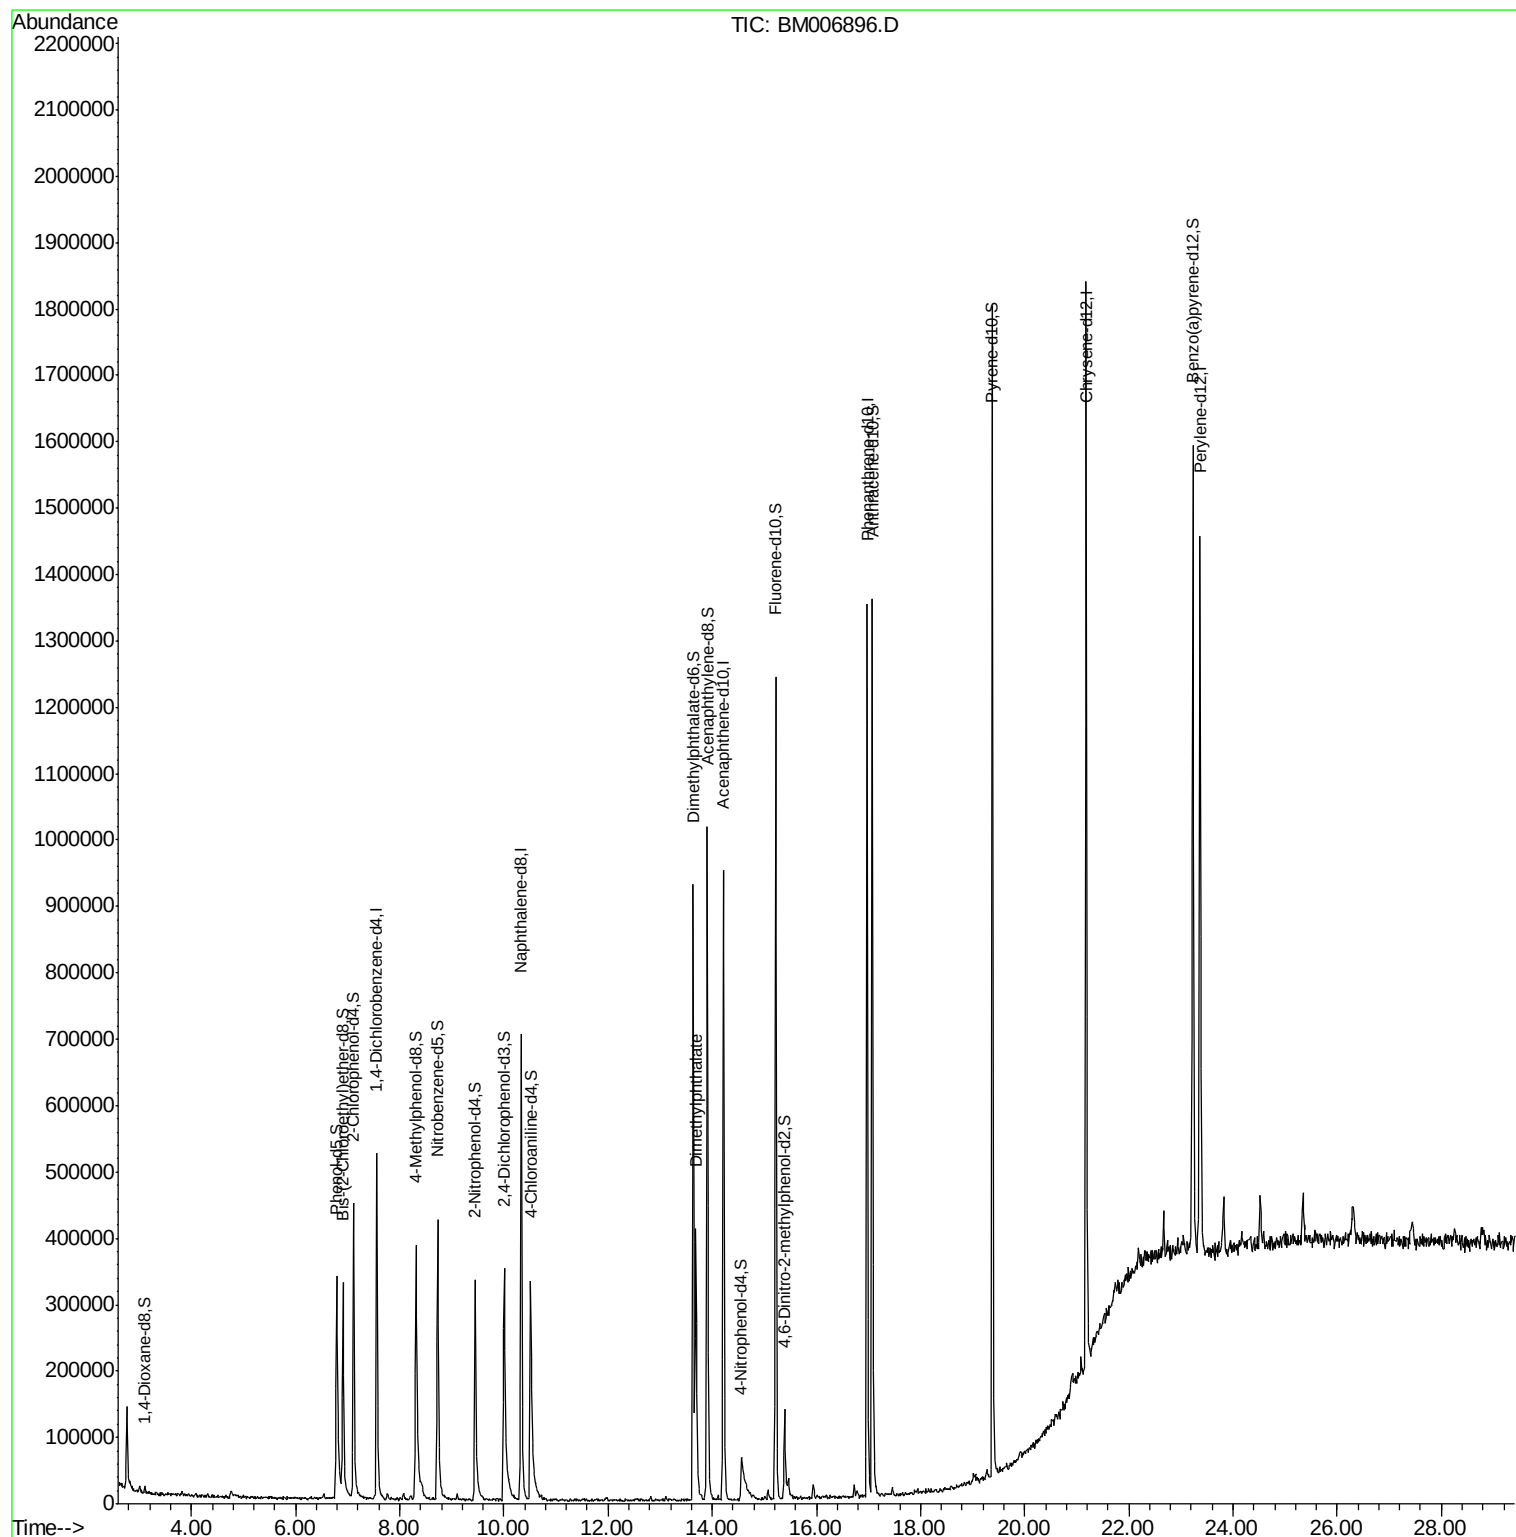

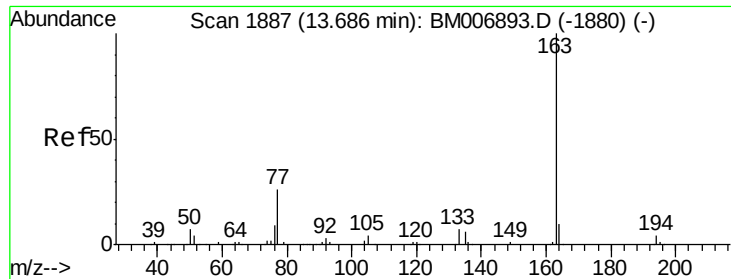

#44

Dimethylphthalate

Concen: 9.66 ng/ul

RT: 13.69 min Scan# 1887

Delta R.T. 0.00 min

Lab File: BM006896.D

Acq: 05 Aug 2016 12:50

Instrument :

BNA_M

ClientSampleId :

BDJN6


Tgt Ion:163 Resp: 247374

Ion Ratio Lower Upper

163 100

194 3.7 3.1 4.7

164 10.6 8.6 12.8

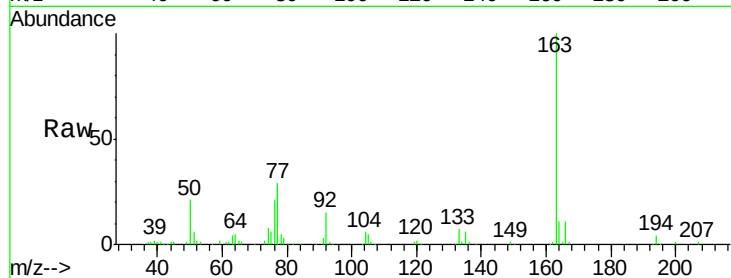

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

