

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006918.D
 Acq On : 06 Aug 2016 02:06
 Operator : UM/SJ
 Sample : H4278-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJR9

Quant Time: Aug 06 03:43:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 06 00:33:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	140084	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	582456	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	349954	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	829903	20.00	ng/ul	0.00
75) Chrysene-d12	21.18	240	953570	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	946245	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	6567	2.58	ng/uL	0.00
5) Phenol-d5	6.78	99	291451	28.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	207690	30.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	235321	28.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	225352	26.87	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	115197	28.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	128563	27.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	215858	22.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	276571	27.31	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	864280	29.98	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	1003457	28.50	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	62571	9.90	ng/ul	0.00
57) Fluorene-d10	15.22	176	738354	27.59	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	84150	15.54	ng/ul	0.00
70) Anthracene-d10	17.07	188	1123991	28.20	ng/ul	0.00
76) Pyrene-d10	19.38	212	1355480	27.79	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.23	264	1310543	28.44	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.69	163	433678	15.14	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006918.D
Acq On : 06 Aug 2016 02:06
Operator : UM/SJ
Sample : H4278-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJR9

Quant Time: Aug 06 03:43:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 06 00:33:11 2016
Response via : Initial Calibration

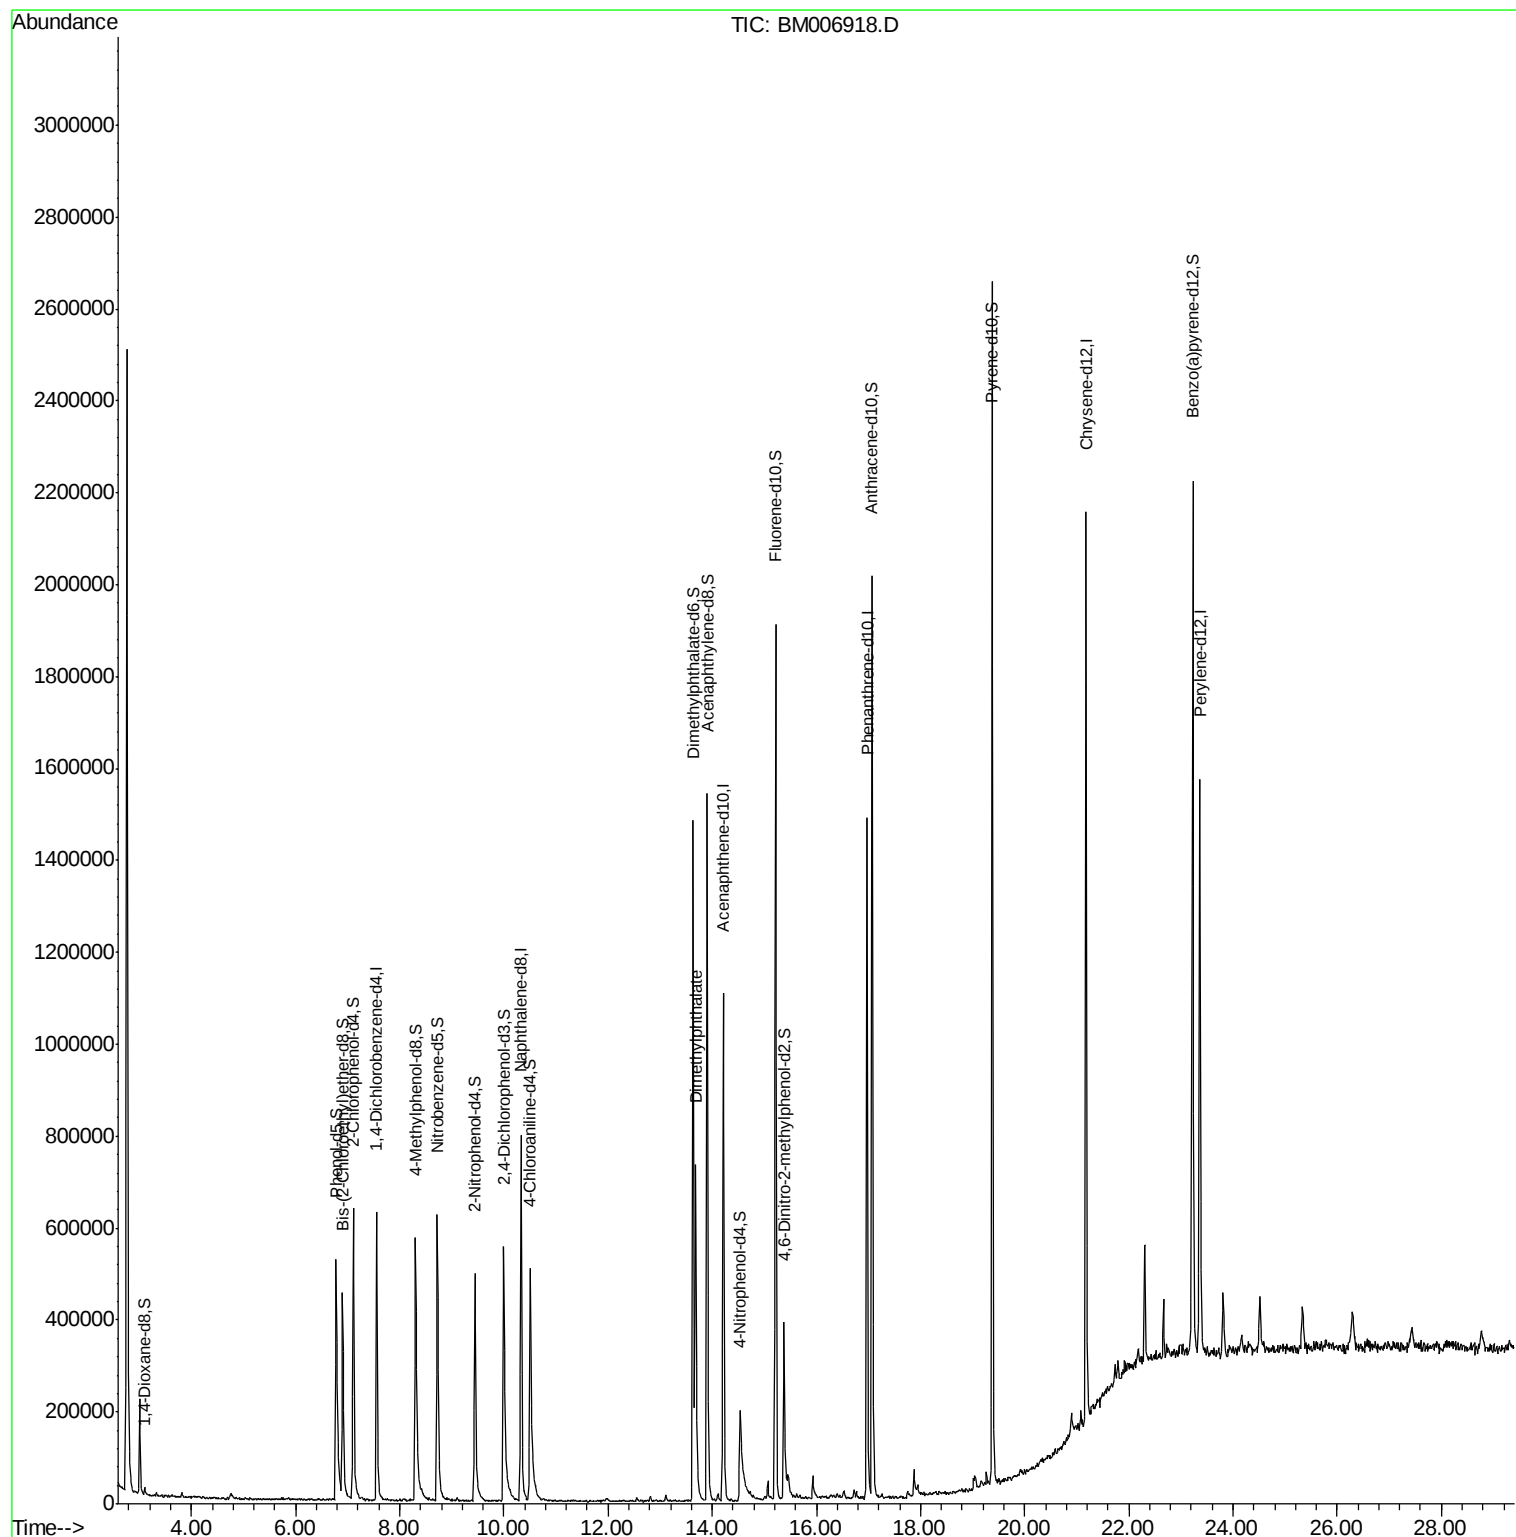

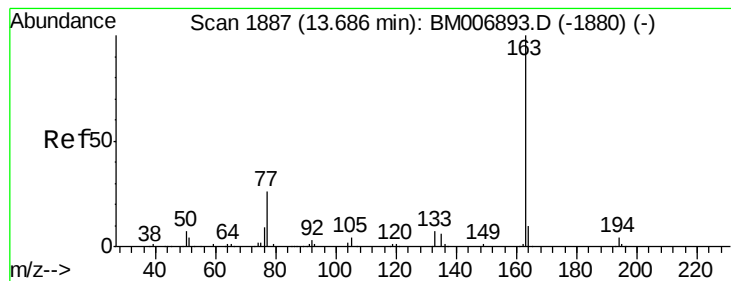

#44

Dimethylphthalate

Concen: 15.14 ng/ul

RT: 13.69 min Scan# 1887

Delta R.T. -0.00 min

Lab File: BM006918.D

Acq: 06 Aug 2016 02:06

Instrument :

BNA_M

ClientSampleId :

BDJR9


Tgt Ion:163 Resp: 433678

Ion Ratio Lower Upper

163 100

194 3.9 3.1 4.7

164 9.4 8.6 12.8

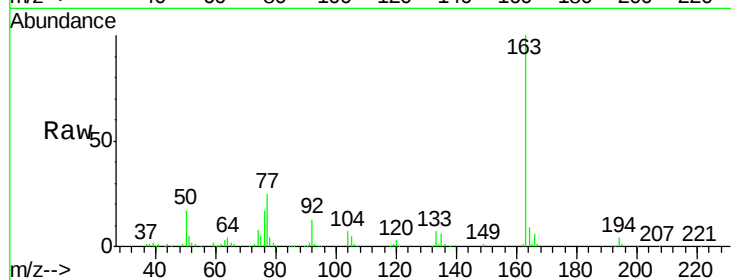

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

