

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006908.D
 Acq On : 05 Aug 2016 20:04
 Operator : UM/SJ
 Sample : H4224-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJL6

Manual Integrations
 APPROVED

sohil
 8/8/2016 7:01:54 PM

Quant Time: Aug 06 01:28:20 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 06 00:33:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	119545	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	519714	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	313827	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	752992	20.00	ng/ul	0.00
75) Chrysene-d12	21.18	240	850012	20.00	ng/ul	0.00
83) Perylene-d12	23.37	264	845523	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.10	96	3467	1.59	ng/uL	0.00
5) Phenol-d5	6.79	99	125394	14.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	99486	16.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	110982	15.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	99158	13.86	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	50655	14.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	58013	13.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	107843m	12.33	ng/ul	0.02
29) 4-Chloroaniline-d4	10.52	131	142167m	15.73	ng/ul	0.02
43) Dimethylphthalate-d6	13.64	166	404608	15.65	ng/ul	0.00
46) Acenaphthylene-d8	13.91	160	476623	15.10	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	42363m	7.47	ng/ul	0.04
57) Fluorene-d10	15.22	176	368642	15.36	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	43092m	8.77	ng/ul	0.01
70) Anthracene-d10	17.07	188	578391	15.99	ng/ul	0.00
76) Pyrene-d10	19.38	212	711075	16.35	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.23	264	686255	16.67	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.69	163	148452	5.78	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006908.D
Acq On : 05 Aug 2016 20:04
Operator : UM/SJ
Sample : H4224-06
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BDJL6

Manual Integrations
APPROVED

sohil
8/8/2016 7:01:54 PM

Quant Time: Aug 06 01:28:20 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 06 00:33:11 2016
Response via : Initial Calibration

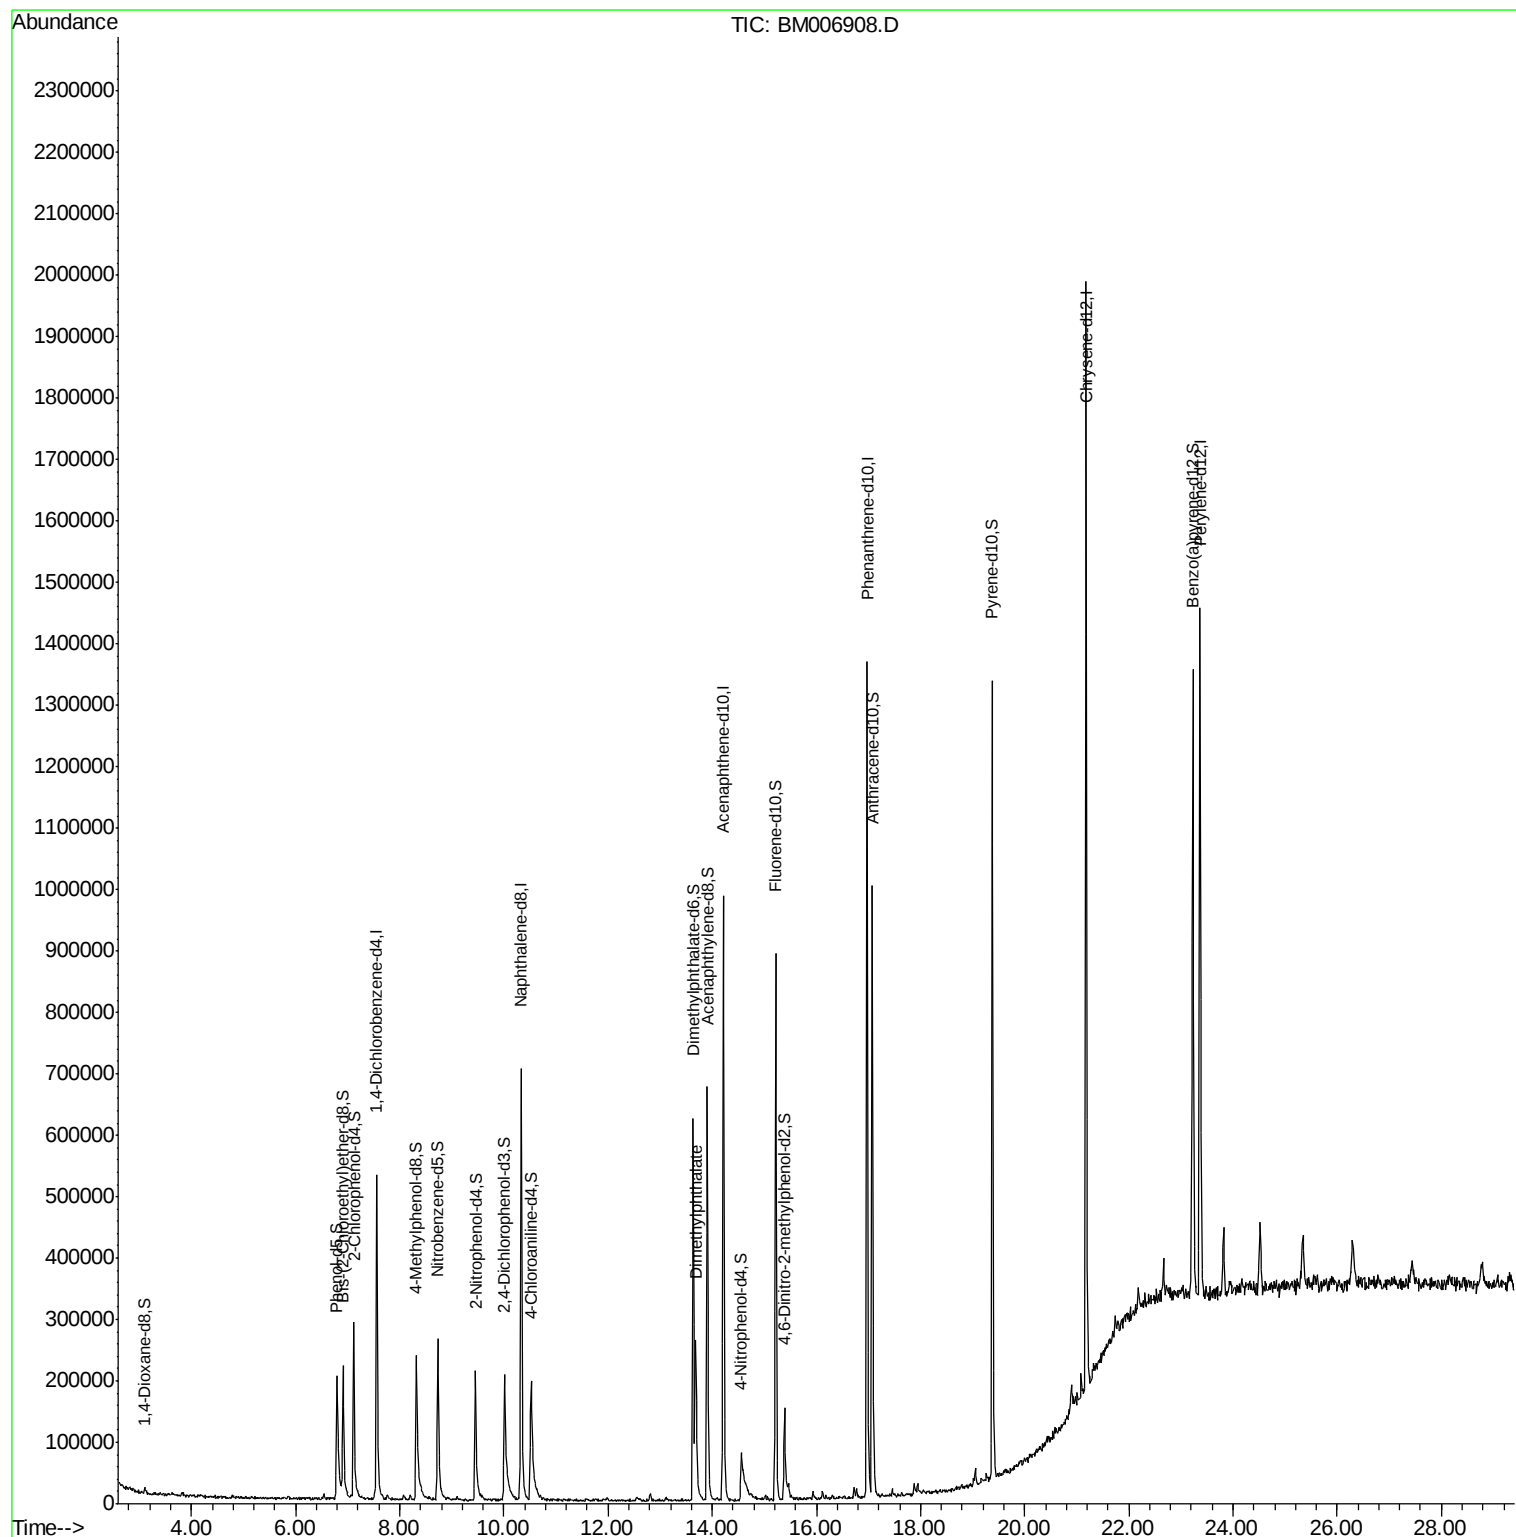

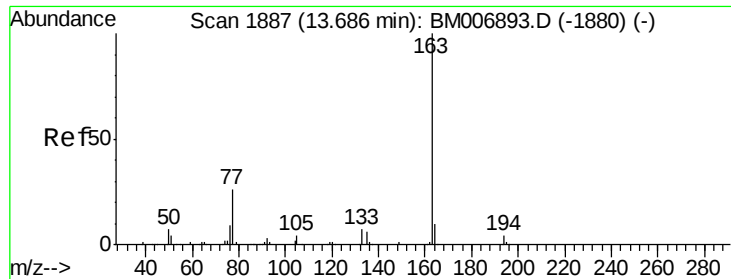

#44
 Dimethylphthalate
 Concen: 5.78 ng/ul
 RT: 13.69 min Scan# 1887
 Delta R.T. -0.00 min
 Lab File: BM006908.D
 Acq: 05 Aug 2016 20:04

Instrument :
 BNA_M
 ClientSampleId :
 BDJL6

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	4.2	3.1	4.7
164	10.2	8.6	12.8

Manual Integrations
 APPROVED

sohil
 8/8/2016 7:01:54 PM

