

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006924.D
 Acq On : 06 Aug 2016 05:45
 Operator : UM/SJ
 Sample : H4278-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJS1

Manual Integrations
 APPROVED

sohil
 8/8/2016 7:02:36 PM

Quant Time: Aug 06 06:34:55 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 06 00:33:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	138292	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	568592	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.21	164	349105	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.97	188	808099	20.00	ng/ul	0.00
75) Chrysene-d12	21.18	240	949796	20.00	ng/ul	0.00
83) Perylene-d12	23.37	264	941662	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	4135	1.64	ng/uL	0.00
5) Phenol-d5	6.79	99	173517	17.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	134292	19.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	146732	18.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	157128m	18.98	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	69757	17.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	80576	17.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	148595m	15.53	ng/ul	0.01
29) 4-Chloroaniline-d4	10.51	131	194939m	19.72	ng/ul	0.00
43) Dimethylphthalate-d6	13.63	166	545513	18.97	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	643595	18.33	ng/ul	0.00
51) 4-Nitrophenol-d4	14.60	143	14784m	2.34	ng/ul	0.07
57) Fluorene-d10	15.22	176	473757	17.75	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	16950	3.21	ng/ul	0.02
70) Anthracene-d10	17.07	188	739105	19.05	ng/ul	0.00
76) Pyrene-d10	19.38	212	887301	18.26	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.23	264	859751	18.75	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	13.69	163	235579	8.24 ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006924.D
Acq On : 06 Aug 2016 05:45
Operator : UM/SJ
Sample : H4278-08
Misc :
ALS Vial : 31 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BDJS1

Manual Integrations
APPROVED

sohil
8/8/2016 7:02:36 PM

Quant Time: Aug 06 06:34:55 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 06 00:33:11 2016
Response via : Initial Calibration

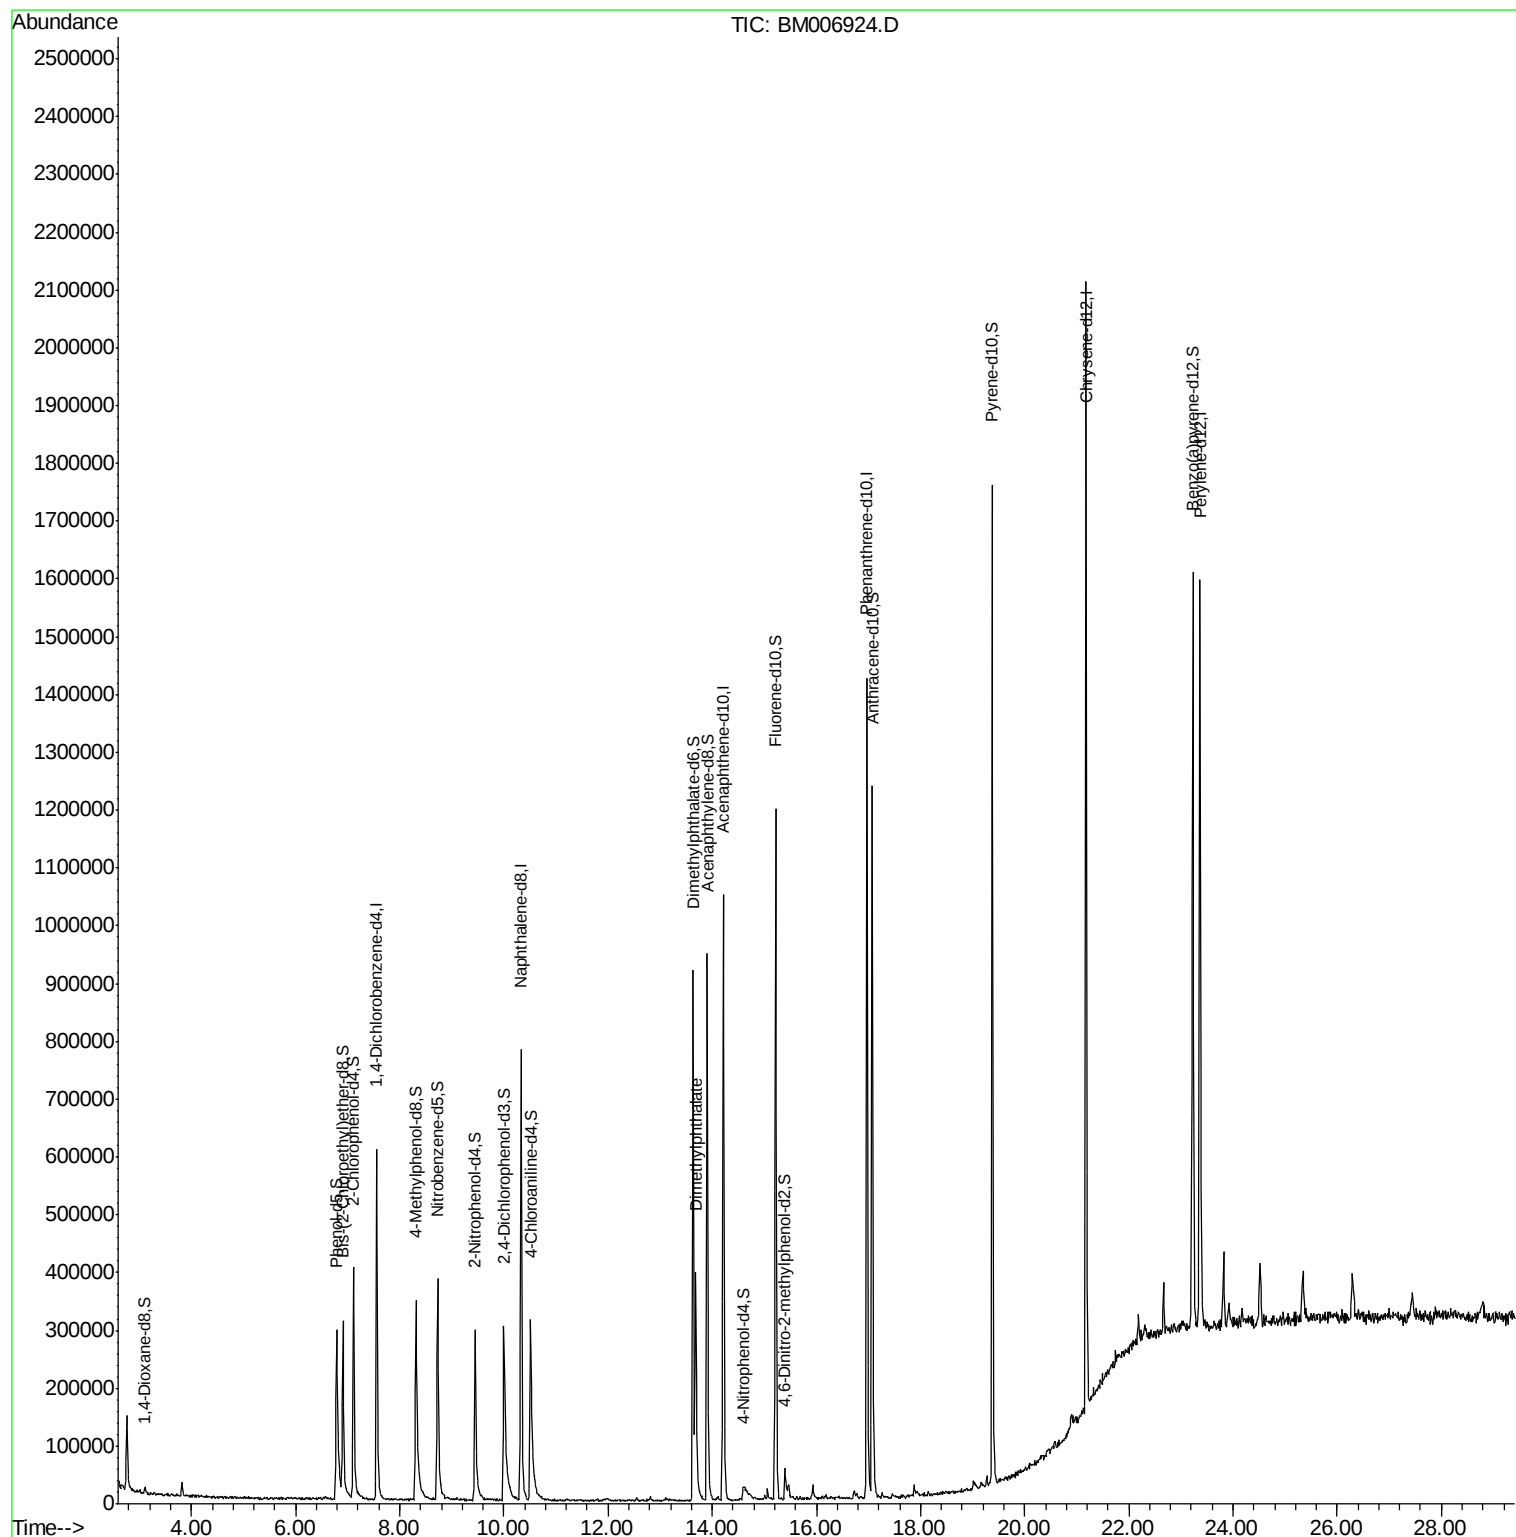

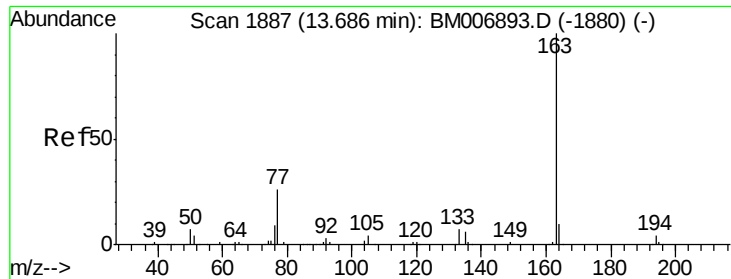

#44
 Dimethylphthalate
 Concen: 8.24 ng/ul
 RT: 13.69 min Scan# 1887
 Delta R.T. 0.00 min
 Lab File: BM006924.D
 Acq: 06 Aug 2016 05:45

Instrument :
 BNA_M
 ClientSampleId :
 BDJS1

Tgt Ion:	163	Resp:	235579
Ion Ratio		Lower	Upper
163	100		
194	4.2	3.1	4.7
164	8.8	8.6	12.8

Manual Integrations
 APPROVED

sohil
 8/8/2016 7:02:36 PM

