

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006894.D
 Acq On : 05 Aug 2016 11:38
 Operator : UM/SJ
 Sample : H4224-10
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJMO

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.758	24	29	45	rVB	657998	1179244	36.06%	3.068%
2	3.810	203	208	215	rBV	34654	57070	1.75%	0.148%
3	6.787	708	714	730	rBV	457615	1059679	32.40%	2.757%
4	6.910	730	735	747	rVB	392559	644721	19.71%	1.677%
5	7.110	761	769	785	rBV	572740	1068696	32.68%	2.781%
6	7.563	838	846	865	rVB	539655	985137	30.12%	2.563%
7	8.310	967	973	994	rBV2	522773	1193474	36.49%	3.105%
8	8.728	1038	1044	1066	rBV	539506	1089746	33.32%	2.835%
9	9.445	1159	1166	1184	rBV	464639	986273	30.16%	2.566%
10	9.998	1254	1260	1286	rBV	503057	1250524	38.24%	3.254%
11	10.339	1309	1318	1333	rBV	675295	1286279	39.33%	3.347%
12	10.510	1341	1347	1361	rBV2	447469	1153313	35.27%	3.001%
13	13.639	1873	1879	1883	rBV	1210709	1765142	53.98%	4.593%
14	13.686	1883	1887	1910	rVB	611447	1150877	35.19%	2.994%
15	13.910	1918	1925	1940	rBV	1323692	2091579	63.96%	5.442%
16	14.216	1970	1977	1992	rBV2	947945	1613058	49.33%	4.197%
17	14.533	2024	2031	2059	rBV	205372	817719	25.00%	2.128%
18	15.221	2141	2148	2161	rVB	1616449	2612675	79.89%	6.798%
19	15.380	2169	2175	2186	rBV3	376926	747669	22.86%	1.945%
20	15.463	2187	2189	2194	rVB4	33828	50273	1.54%	0.131%
21	15.933	2264	2269	2271	rBV2	34923	43584	1.33%	0.113%
22	16.727	2399	2404	2407	rBV2	30163	40821	1.25%	0.106%
23	16.974	2439	2446	2457	rBV	1298120	1976253	60.43%	5.142%
24	17.074	2457	2463	2480	rVB	1797200	2849924	87.15%	7.415%
25	19.380	2849	2855	2867	rBV	2229463	3270255	100.00%	8.509%
26	20.892	3109	3112	3113	rBV3	54128	52725	1.61%	0.137%
27	21.186	3157	3162	3173	rBV2	1737049	2410113	73.70%	6.271%
28	23.233	3504	3510	3522	rVB	1541991	3006380	91.93%	7.822%
29	23.374	3528	3534	3543	rVB	994990	1980695	60.57%	5.154%


Sum of corrected areas: 38433898

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006894.D
Acq On : 05 Aug 2016 11:38
Operator : UM/SJ
Sample : H4224-10
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BDJM0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

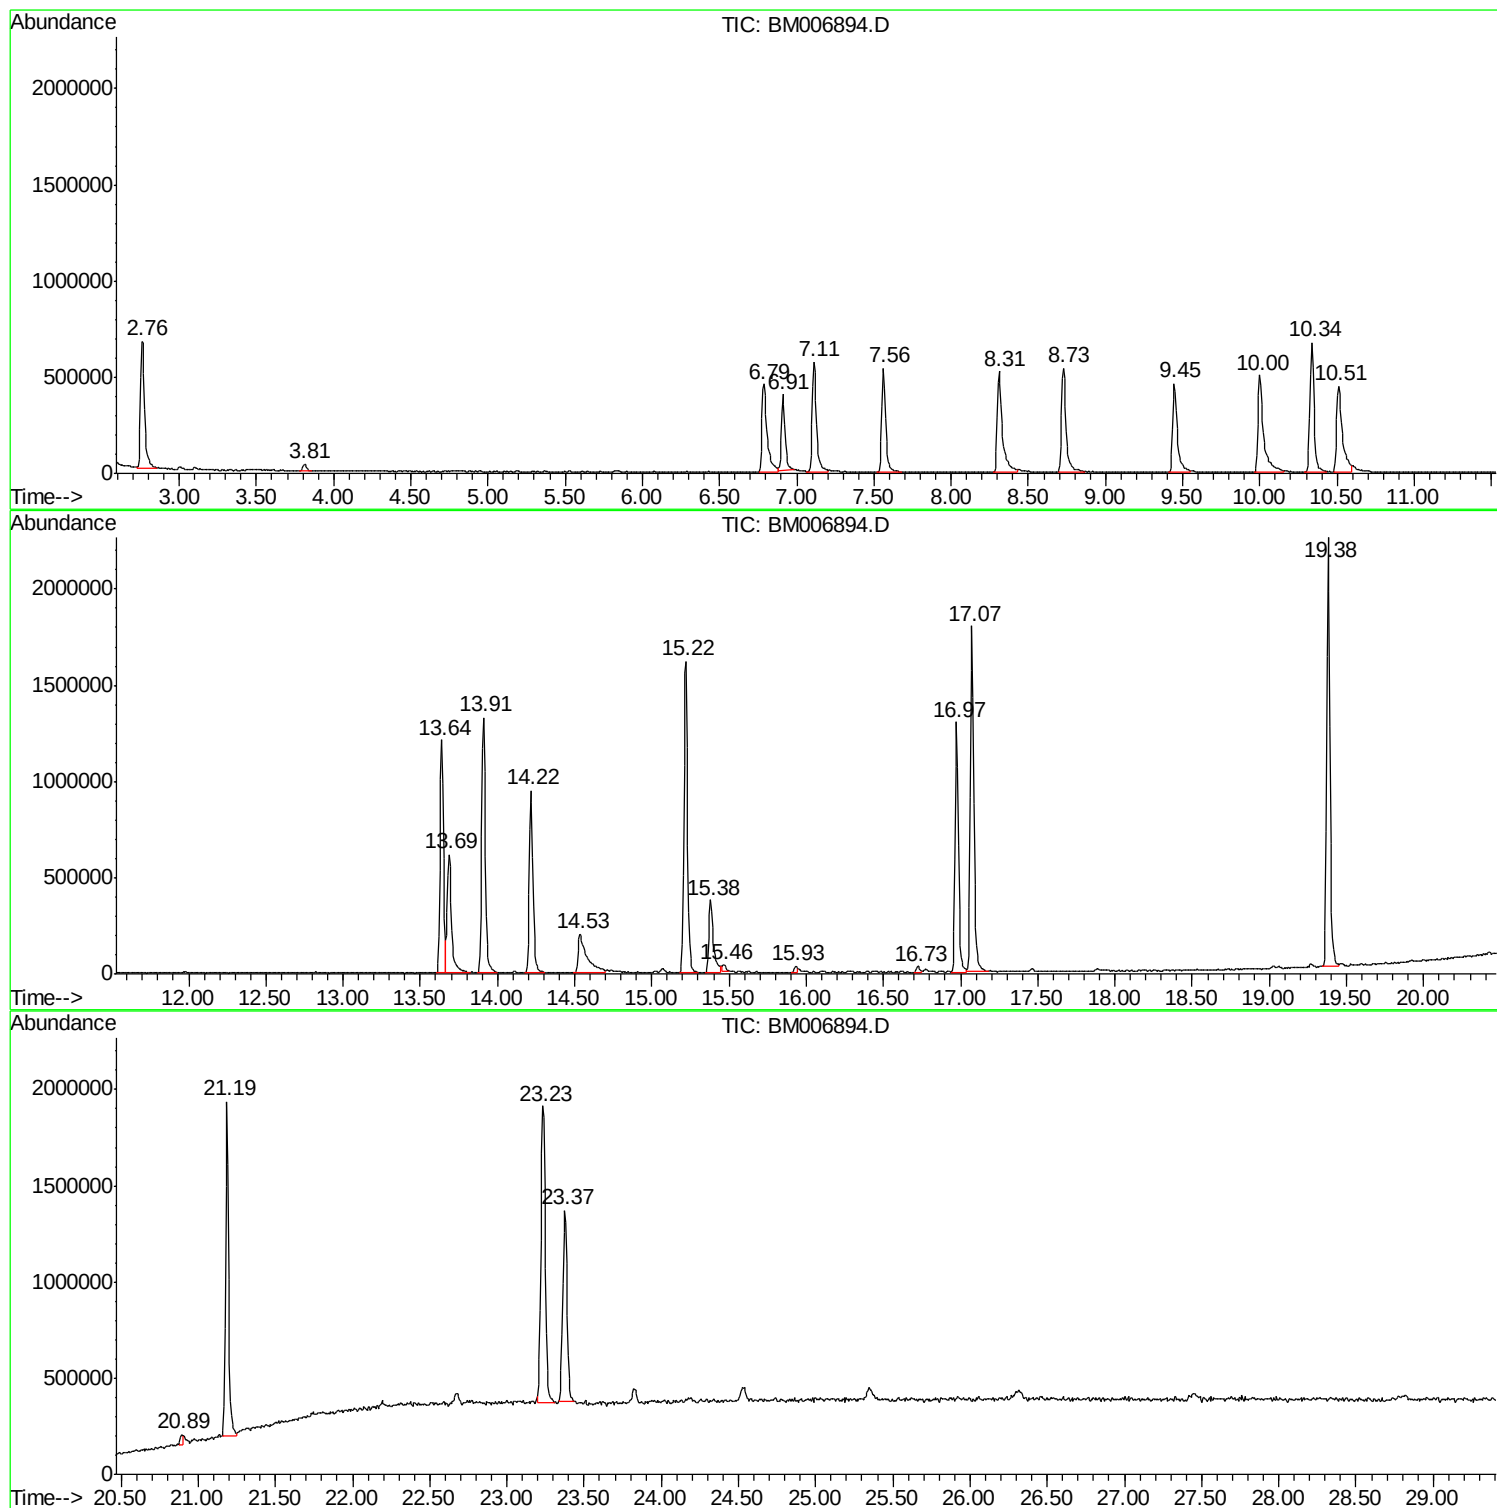

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006894.D
Acq On : 05 Aug 2016 11:38
Operator : UM/SJ
Sample : H4224-10
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJM0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006894.D
Acq On : 05 Aug 2016 11:38
Operator : UM/SJ
Sample : H4224-10
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJM0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc