

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006896.D
 Acq On : 05 Aug 2016 12:50
 Operator : UM/SJ
 Sample : H4224-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJN6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.763	24	30	37	rBV	122724	219207	8.38%	0.708%
2	4.757	364	369	375	rBV6	10314	27609	1.06%	0.089%
3	6.787	707	714	728	rBV	335180	816476	31.21%	2.638%
4	6.910	730	735	750	rVB	318250	550909	21.06%	1.780%
5	7.110	763	769	784	rBV	440190	816859	31.23%	2.639%
6	7.557	839	845	860	rVB	515549	928923	35.51%	3.001%
7	8.310	967	973	986	rBV2	381471	885548	33.86%	2.861%
8	8.728	1037	1044	1062	rBV	421945	861866	32.95%	2.784%
9	9.445	1160	1166	1186	rBV2	330562	736785	28.17%	2.380%
10	10.004	1253	1261	1275	rBV	349128	921930	35.25%	2.978%
11	10.333	1309	1317	1336	rBV	700666	1284908	49.12%	4.151%
12	10.516	1341	1348	1377	rBV2	328691	956893	36.58%	3.091%
13	13.639	1873	1879	1883	rBV	927425	1402981	53.64%	4.533%
14	13.686	1883	1887	1900	rVB	400837	774925	29.63%	2.504%
15	13.910	1919	1925	1941	rVB	1012035	1642548	62.80%	5.307%
16	14.216	1970	1977	1993	rBV2	948690	1641565	62.76%	5.303%
17	14.563	2030	2036	2049	rBV3	64041	258667	9.89%	0.836%
18	15.215	2141	2147	2160	rBV	1238801	2060152	78.76%	6.656%
19	15.386	2171	2176	2186	rBV2	135263	298727	11.42%	0.965%
20	15.463	2187	2189	2194	rVB5	25424	36551	1.40%	0.118%
21	15.933	2265	2269	2271	rBV2	20081	27840	1.06%	0.090%
22	16.727	2400	2404	2408	rBV2	18857	29768	1.14%	0.096%
23	16.974	2440	2446	2456	rBV	1346707	2011441	76.90%	6.498%
24	17.074	2456	2463	2473	rVV2	1345119	2207886	84.41%	7.133%
25	19.380	2849	2855	2864	rBV	1764674	2615681	100.00%	8.451%
26	21.180	3156	3161	3173	rBV2	1633213	2424156	92.68%	7.832%
27	23.233	3503	3510	3523	rVB2	1218179	2450099	93.67%	7.916%
28	23.368	3527	3533	3543	rVB	1071848	2061960	78.83%	6.662%


Sum of corrected areas: 30952860

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006896.D
Acq On : 05 Aug 2016 12:50
Operator : UM/SJ
Sample : H4224-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJN6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

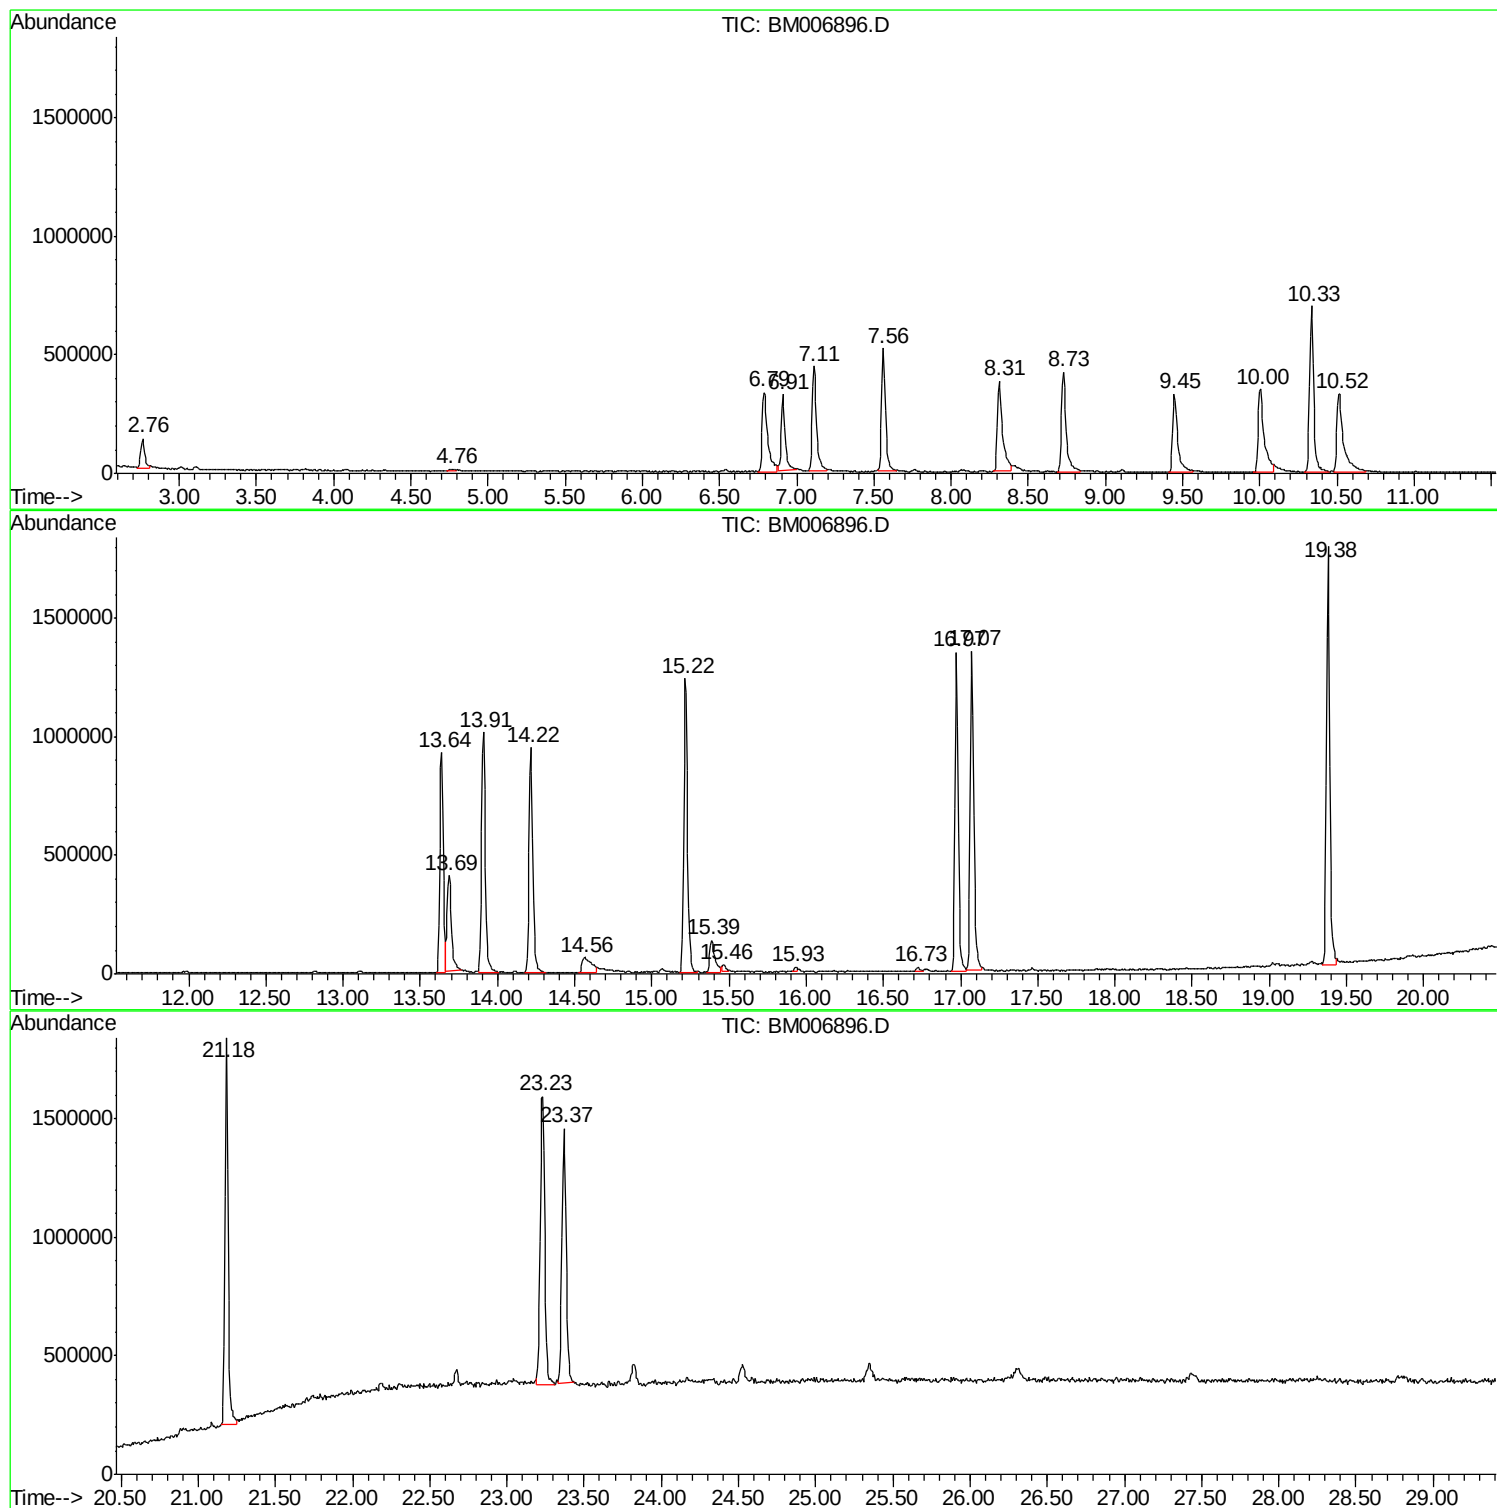

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006896.D
Acq On : 05 Aug 2016 12:50
Operator : UM/SJ
Sample : H4224-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJN6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006896.D
Acq On : 05 Aug 2016 12:50
Operator : UM/SJ
Sample : H4224-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJN6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc