

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006902.D
 Acq On : 05 Aug 2016 16:27
 Operator : UM/SJ
 Sample : H4224-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJP2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.763	24	30	43	rVB	697999	1224604	29.03%	2.556%
2	6.781	707	713	729	rBV	634705	1381543	32.75%	2.884%
3	6.910	729	735	748	rVB	515944	876693	20.78%	1.830%
4	7.110	762	769	782	rBV	736128	1356340	32.15%	2.831%
5	7.557	839	845	861	rBV	602204	1097246	26.01%	2.290%
6	8.304	966	972	1003	rBV	730636	1621256	38.43%	3.384%
7	8.722	1037	1043	1064	rBV	714941	1442781	34.20%	3.011%
8	9.439	1159	1165	1185	rBV	611871	1284455	30.45%	2.681%
9	9.992	1253	1259	1282	rBV2	655811	1632065	38.69%	3.406%
10	10.333	1310	1317	1338	rVB	821928	1449878	34.37%	3.026%
11	10.504	1338	1346	1375	rBV	642521	1660607	39.36%	3.466%
12	13.633	1873	1878	1883	rBV	1545030	2354698	55.82%	4.915%
13	13.686	1883	1887	1906	rVB	742837	1342759	31.83%	2.803%
14	13.904	1918	1924	1942	rVB	1640562	2713036	64.31%	5.663%
15	14.215	1969	1977	1991	rBV2	1112279	1845626	43.75%	3.852%
16	14.521	2024	2029	2052	rBV3	318899	1146526	27.18%	2.393%
17	15.062	2117	2121	2127	rBV	27407	42279	1.00%	0.088%
18	15.215	2140	2147	2160	rBV	2197888	3367599	79.82%	7.029%
19	15.374	2168	2174	2185	rBV	541735	1047065	24.82%	2.185%
20	15.462	2185	2189	2195	rVB6	41578	85804	2.03%	0.179%
21	15.933	2265	2269	2276	rBV	43857	82383	1.95%	0.172%
22	16.721	2396	2403	2408	rBV2	45417	68980	1.64%	0.144%
23	16.974	2440	2446	2456	rBV	1450690	2199585	52.14%	4.591%
24	17.074	2456	2463	2479	rVB	2263751	3623111	85.88%	7.562%
25	19.380	2849	2855	2867	rBV	2930621	4218732	100.00%	8.805%
26	20.897	3108	3113	3118	rBV7	72222	156544	3.71%	0.327%
27	21.186	3157	3162	3171	rBV	1807178	2543566	60.29%	5.309%
28	23.233	3503	3510	3519	rVB2	2057910	3846224	91.17%	8.028%
29	23.368	3527	3533	3541	rBV	1133879	2199368	52.13%	4.590%


Sum of corrected areas: 47911353

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006902.D
Acq On : 05 Aug 2016 16:27
Operator : UM/SJ
Sample : H4224-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJP2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

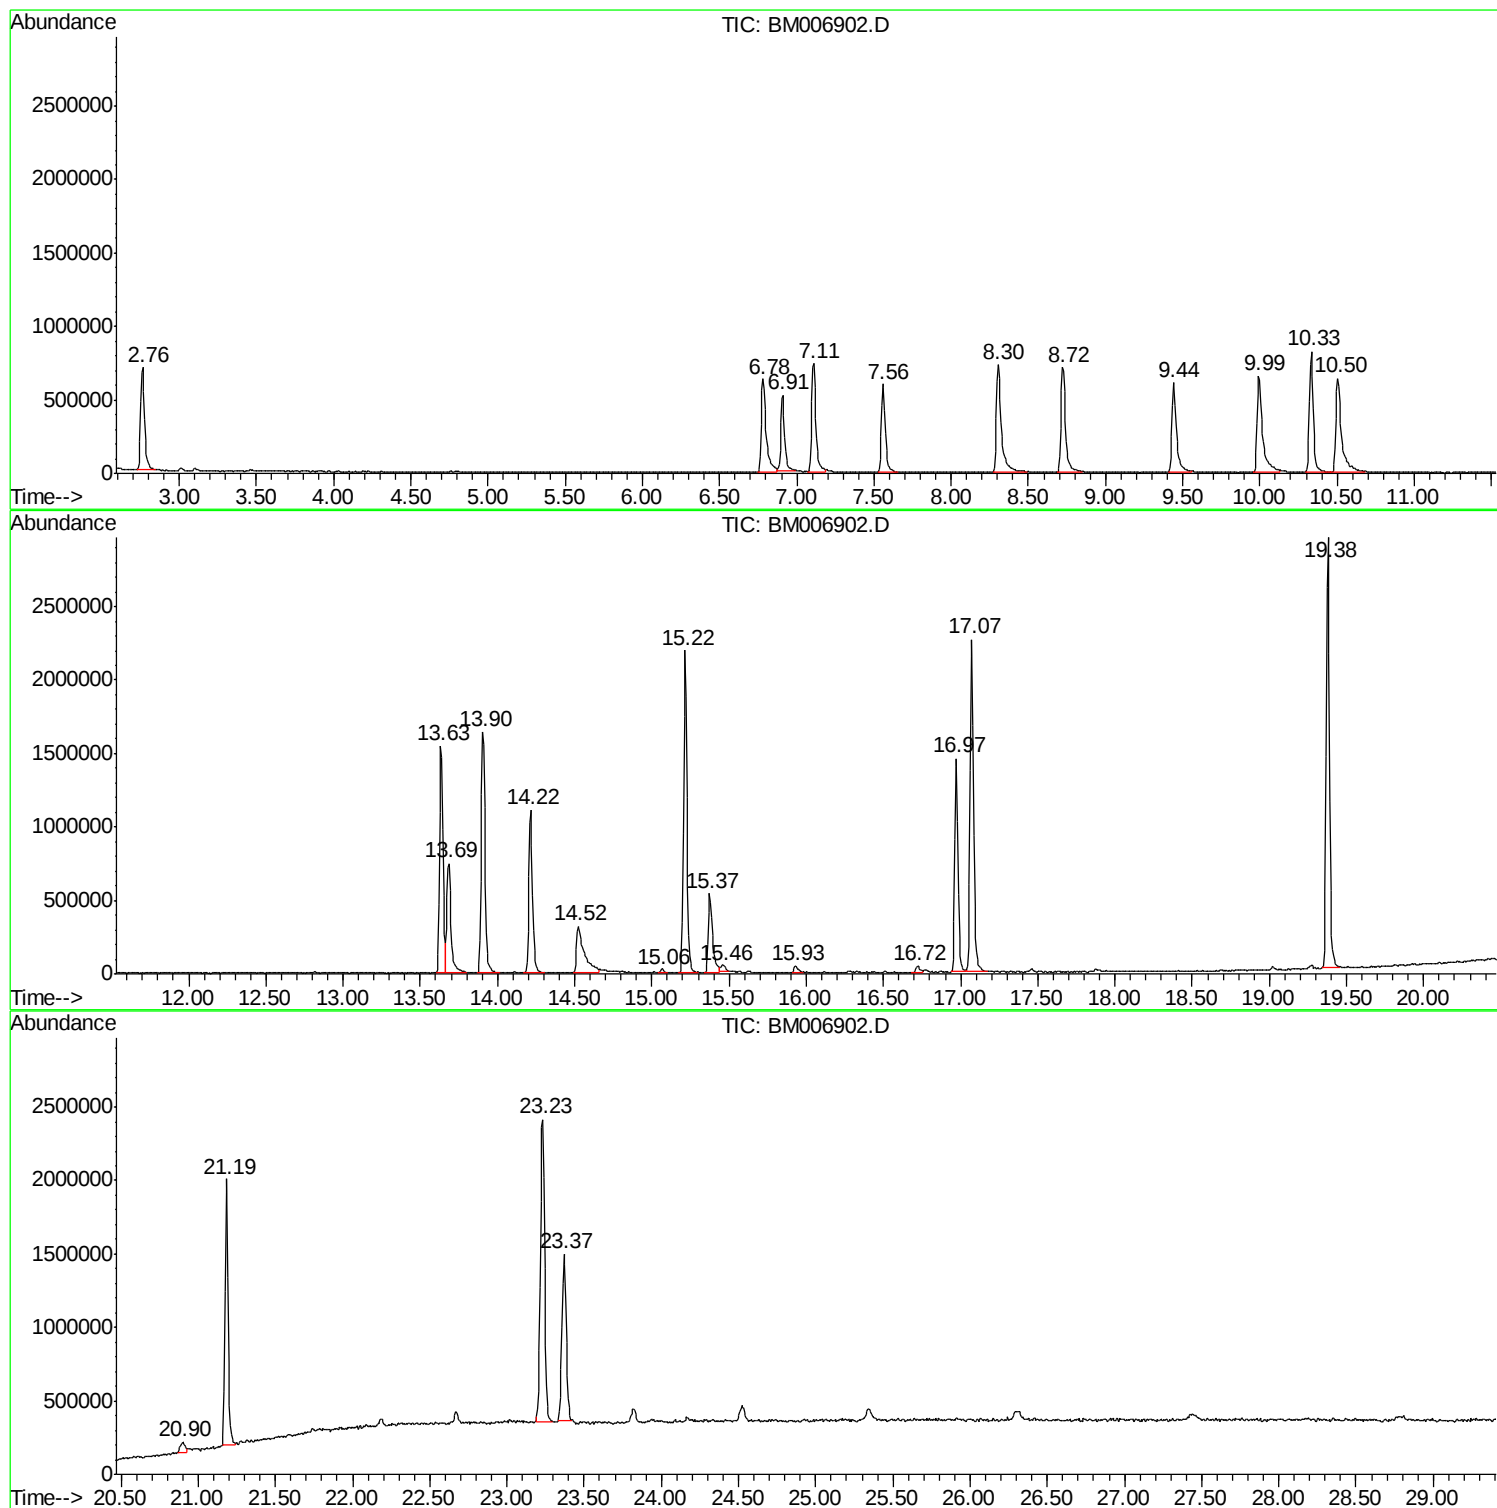

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006902.D
Acq On : 05 Aug 2016 16:27
Operator : UM/SJ
Sample : H4224-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJP2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006902.D
Acq On : 05 Aug 2016 16:27
Operator : UM/SJ
Sample : H4224-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJP2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc