

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006904.D
 Acq On : 05 Aug 2016 17:39
 Operator : UM/SJ
 Sample : H4224-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.793	707	715	728	rBV3	204163	523187	21.21%	2.166%
2	6.910	731	735	746	rVB	194434	350617	14.22%	1.451%
3	7.116	763	770	779	rBV	271533	533610	21.64%	2.209%
4	7.557	839	845	860	rVB	556422	997668	40.45%	4.130%
5	8.316	969	974	993	rBV2	217804	582761	23.63%	2.412%
6	8.728	1037	1044	1063	rBV	253417	574355	23.29%	2.377%
7	9.451	1161	1167	1189	rBV2	199844	484590	19.65%	2.006%
8	10.010	1256	1262	1279	rBV3	194790	580085	23.52%	2.401%
9	10.334	1311	1317	1335	rBV	731193	1366558	55.41%	5.657%
10	10.516	1342	1348	1369	rBV	200428	623728	25.29%	2.582%
11	13.639	1873	1879	1883	rBV	610526	927518	37.61%	3.839%
12	13.686	1883	1887	1902	rVB	279801	547946	22.22%	2.268%
13	13.910	1918	1925	1940	rBV	630386	1062636	43.09%	4.399%
14	14.216	1969	1977	1992	rBV2	1013229	1722060	69.82%	7.128%
15	14.569	2031	2037	2040	rBV4	57298	105703	4.29%	0.438%
16	15.222	2141	2148	2160	rBV	790130	1371734	55.62%	5.678%
17	15.386	2171	2176	2186	rBV4	99452	241171	9.78%	0.998%
18	16.974	2439	2446	2457	rBV	1377400	2101721	85.22%	8.700%
19	17.074	2457	2463	2476	rVB	889096	1439254	58.36%	5.958%
20	19.274	2831	2837	2841	rBV6	13758	30970	1.26%	0.128%
21	19.380	2849	2855	2866	rBV	1139550	1737065	70.43%	7.190%
22	21.180	3156	3161	3170	rBV	1691331	2466367	100.00%	10.209%
23	23.233	3503	3510	3519	rVB	839692	1609587	65.26%	6.663%
24	23.368	3527	3533	3546	rVB	1073829	2177313	88.28%	9.013%


Sum of corrected areas: 24158204

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006904.D
Acq On : 05 Aug 2016 17:39
Operator : UM/SJ
Sample : H4224-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJL3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

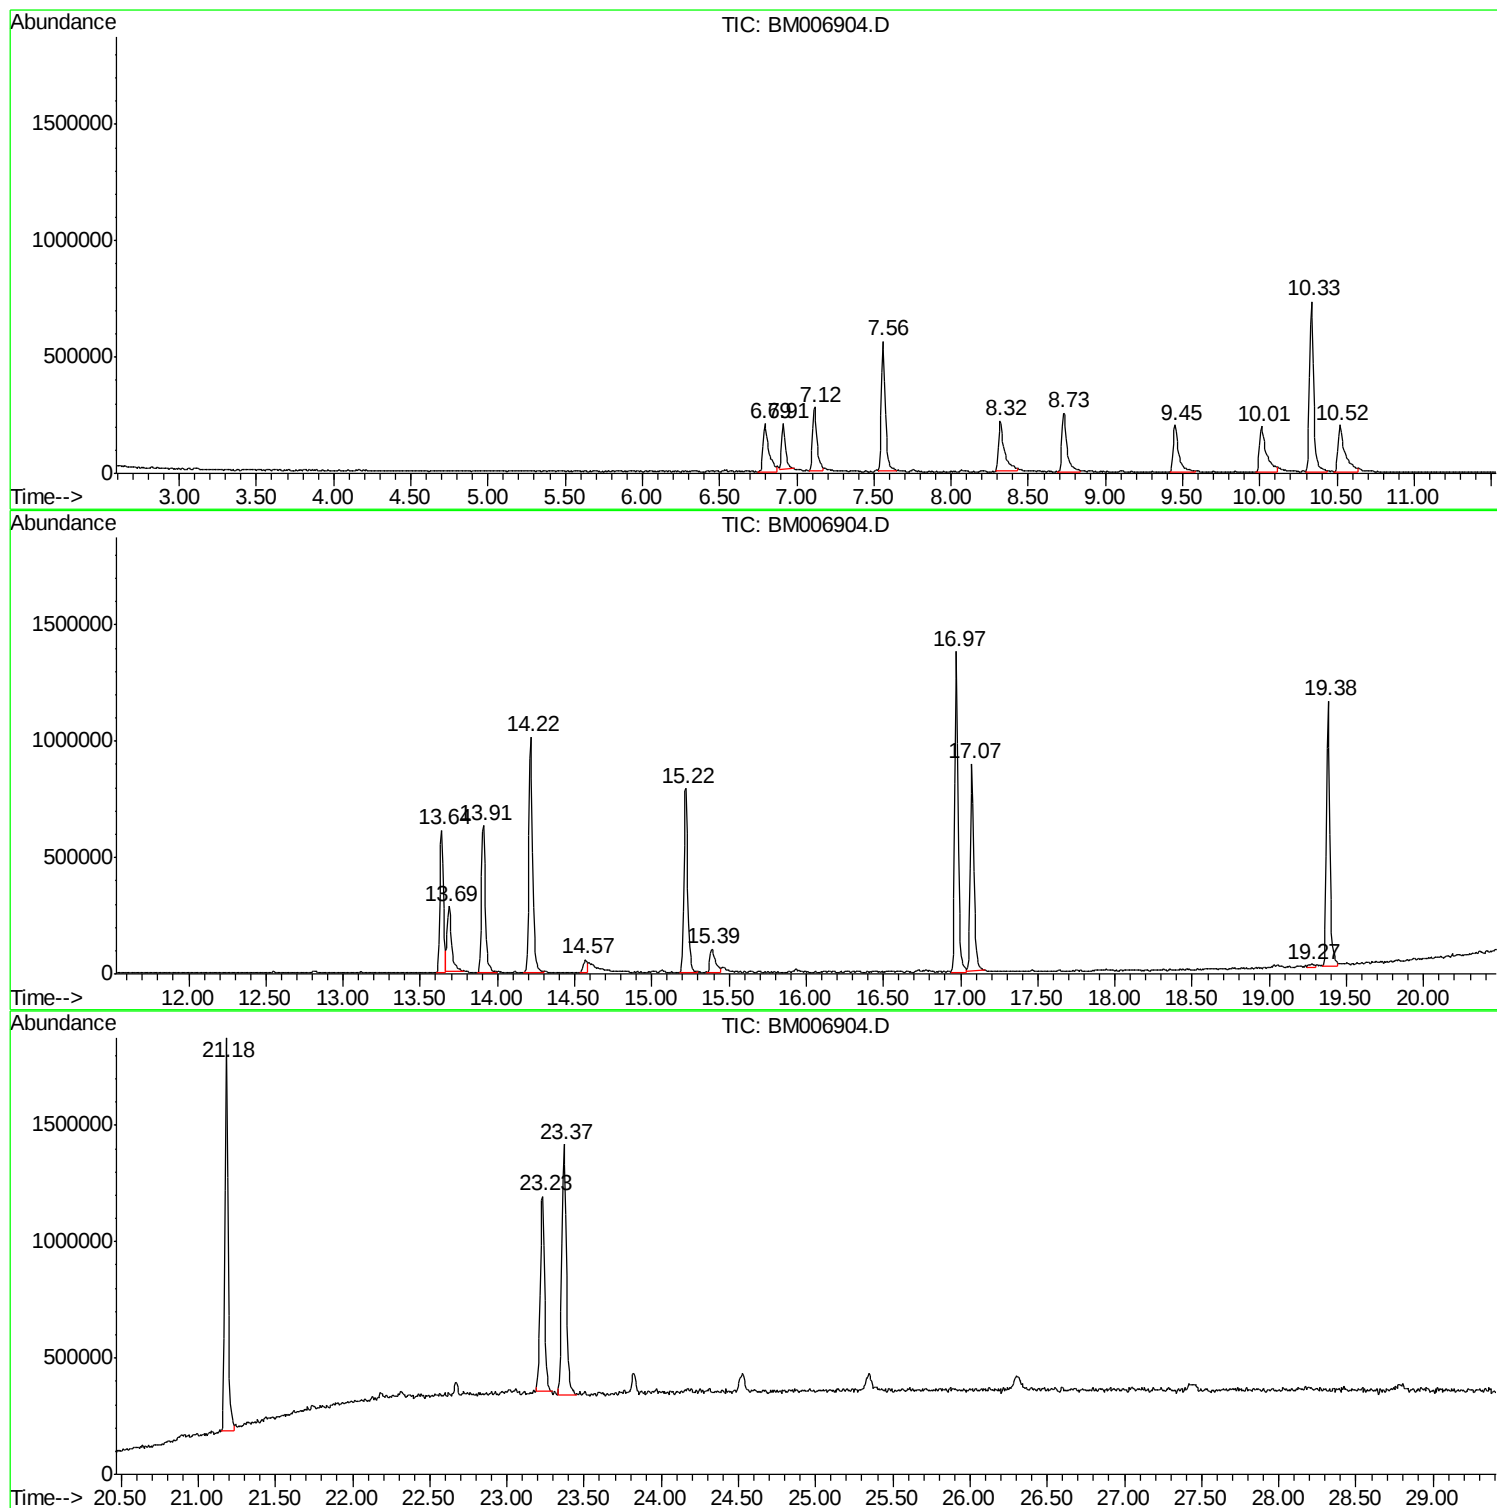

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006904.D
Acq On : 05 Aug 2016 17:39
Operator : UM/SJ
Sample : H4224-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJL3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006904.D
Acq On : 05 Aug 2016 17:39
Operator : UM/SJ
Sample : H4224-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJL3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc