

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006909.D
 Acq On : 05 Aug 2016 20:40
 Operator : UM/SJ
 Sample : H4224-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJL7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.763	24	30	36	rBV	117249	214086	7.57%	0.651%
2	6.787	705	714	729	rBV2	359752	875047	30.93%	2.662%
3	6.910	730	735	748	rVB	332398	569592	20.13%	1.733%
4	7.110	761	769	789	rBV	467914	907922	32.09%	2.762%
5	7.557	840	845	858	rVB	533762	945613	33.42%	2.876%
6	8.310	967	973	988	rBV2	404365	966613	34.17%	2.940%
7	8.728	1037	1044	1062	rBV	452815	929806	32.86%	2.828%
8	9.445	1160	1166	1184	rBV2	340240	781310	27.62%	2.377%
9	10.004	1254	1261	1287	rBV2	350910	1046945	37.01%	3.185%
10	10.333	1309	1317	1330	rBV	703362	1275203	45.07%	3.879%
11	10.516	1342	1348	1364	rBV2	253620	740278	26.17%	2.252%
12	13.633	1873	1878	1883	rBV	937746	1495603	52.86%	4.549%
13	13.686	1883	1887	1903	rVB	456460	863940	30.54%	2.628%
14	13.904	1918	1924	1940	rBV	1026817	1730592	61.17%	5.264%
15	14.216	1970	1977	1992	rBV2	944693	1613776	57.04%	4.909%
16	14.545	2027	2033	2052	rBV4	128065	536424	18.96%	1.632%
17	15.215	2141	2147	2161	rVB	1408020	2210588	78.14%	6.724%
18	15.380	2170	2175	2186	rBV2	224549	500395	17.69%	1.522%
19	15.463	2186	2189	2195	rVB5	27799	50594	1.79%	0.154%
20	15.927	2262	2268	2276	rBV5	15295	31666	1.12%	0.096%
21	16.974	2440	2446	2457	rBV	1285538	1961749	69.34%	5.967%
22	17.074	2457	2463	2478	rVB	1399428	2334454	82.51%	7.101%
23	19.380	2849	2855	2868	rBV	1893879	2829182	100.00%	8.606%
24	21.180	3156	3161	3172	rBV	1650166	2434927	86.06%	7.406%
25	23.227	3502	3509	3522	rVB2	1412444	2810659	99.35%	8.549%
26	23.368	3527	3533	3545	rVB	1129032	2218850	78.43%	6.749%


Sum of corrected areas: 32875814

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006909.D
Acq On : 05 Aug 2016 20:40
Operator : UM/SJ
Sample : H4224-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJL7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

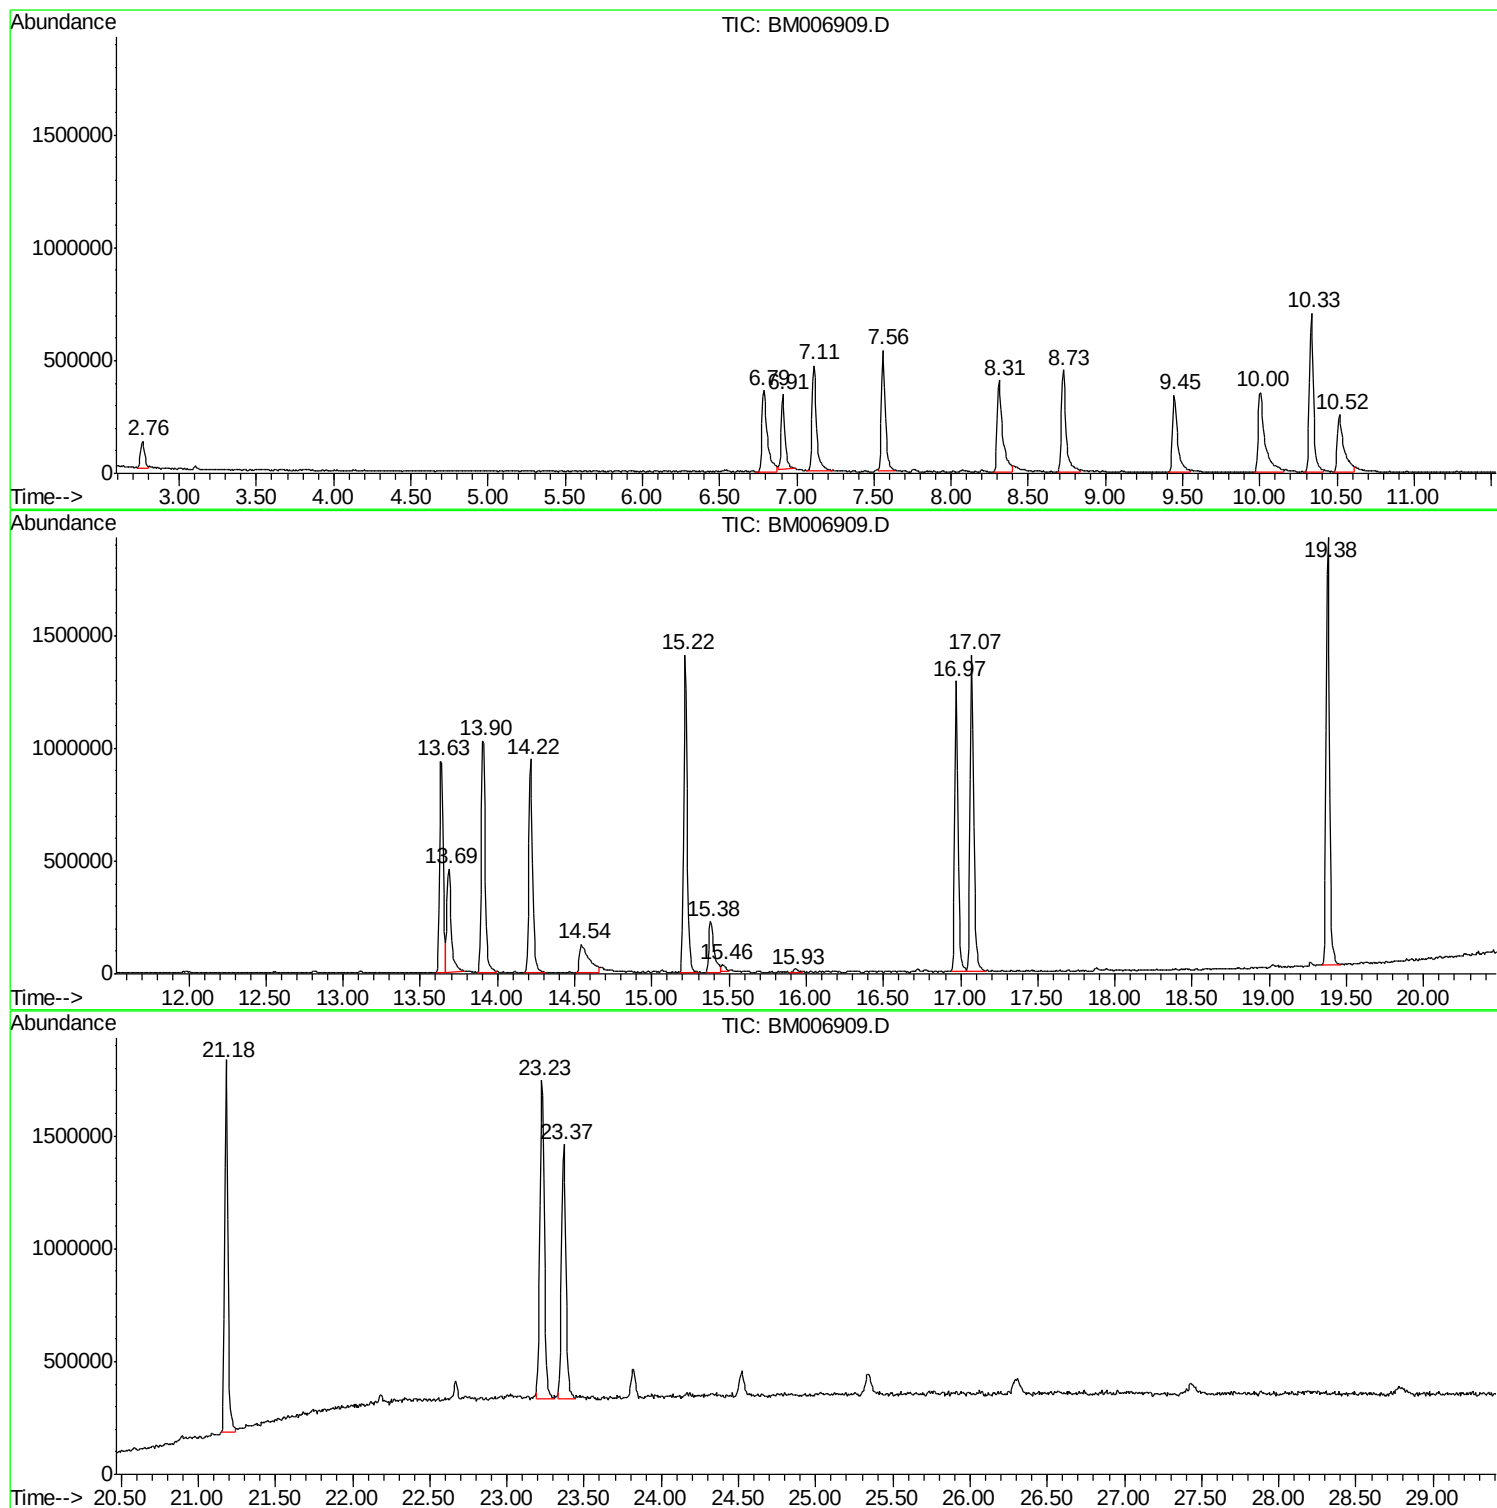

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006909.D
Acq On : 05 Aug 2016 20:40
Operator : UM/SJ
Sample : H4224-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJL7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006909.D
Acq On : 05 Aug 2016 20:40
Operator : UM/SJ
Sample : H4224-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJL7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc