

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006920.D
 Acq On : 06 Aug 2016 03:20
 Operator : UM/SJ
 Sample : H4278-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJS0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.763	24	30	51	rVB	60378105	84759467	100.00%	62.714%
2	6.775	707	712	728	rBV	733928	1614717	1.91%	1.195%
3	6.904	728	734	747	rVB	603094	1010995	1.19%	0.748%
4	7.104	761	768	787	rBV	854489	1585362	1.87%	1.173%
5	7.557	839	845	859	rBV	676564	1178854	1.39%	0.872%
6	8.298	966	971	995	rBV	809961	1790308	2.11%	1.325%
7	8.722	1037	1043	1066	rBV	841848	1602358	1.89%	1.186%
8	9.439	1158	1165	1186	rBV	693306	1440765	1.70%	1.066%
9	9.992	1253	1259	1289	rBV	726760	1859152	2.19%	1.376%
10	10.333	1308	1317	1332	rBV	793225	1502811	1.77%	1.112%
11	10.504	1339	1346	1374	rBV	649015	1670256	1.97%	1.236%
12	13.633	1871	1878	1883	rBV	1743189	2577109	3.04%	1.907%
13	13.680	1883	1886	1903	rVB	784375	1319542	1.56%	0.976%
14	13.904	1915	1924	1937	rBV	1864289	2985242	3.52%	2.209%
15	14.215	1968	1977	1991	rBV2	1106761	1895983	2.24%	1.403%
16	14.521	2023	2029	2060	rBV3	329573	1228750	1.45%	0.909%
17	15.215	2141	2147	2160	rVB	2345764	3651659	4.31%	2.702%
18	15.374	2168	2174	2184	rBV2	591533	1117042	1.32%	0.827%
19	16.974	2440	2446	2456	rBV2	1466418	2288705	2.70%	1.693%
20	17.068	2456	2462	2481	rVB	2418685	3922038	4.63%	2.902%
21	19.380	2849	2855	2867	rBV	3146070	4470267	5.27%	3.308%
22	21.186	3156	3162	3172	rBV	1907649	2818686	3.33%	2.086%
23	23.232	3503	3510	3523	rVB2	2196289	4237524	5.00%	3.135%
24	23.374	3527	3534	3546	rVB	1270025	2625001	3.10%	1.942%


Sum of corrected areas: 135152593

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006920.D
Acq On : 06 Aug 2016 03:20
Operator : UM/SJ
Sample : H4278-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJS0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

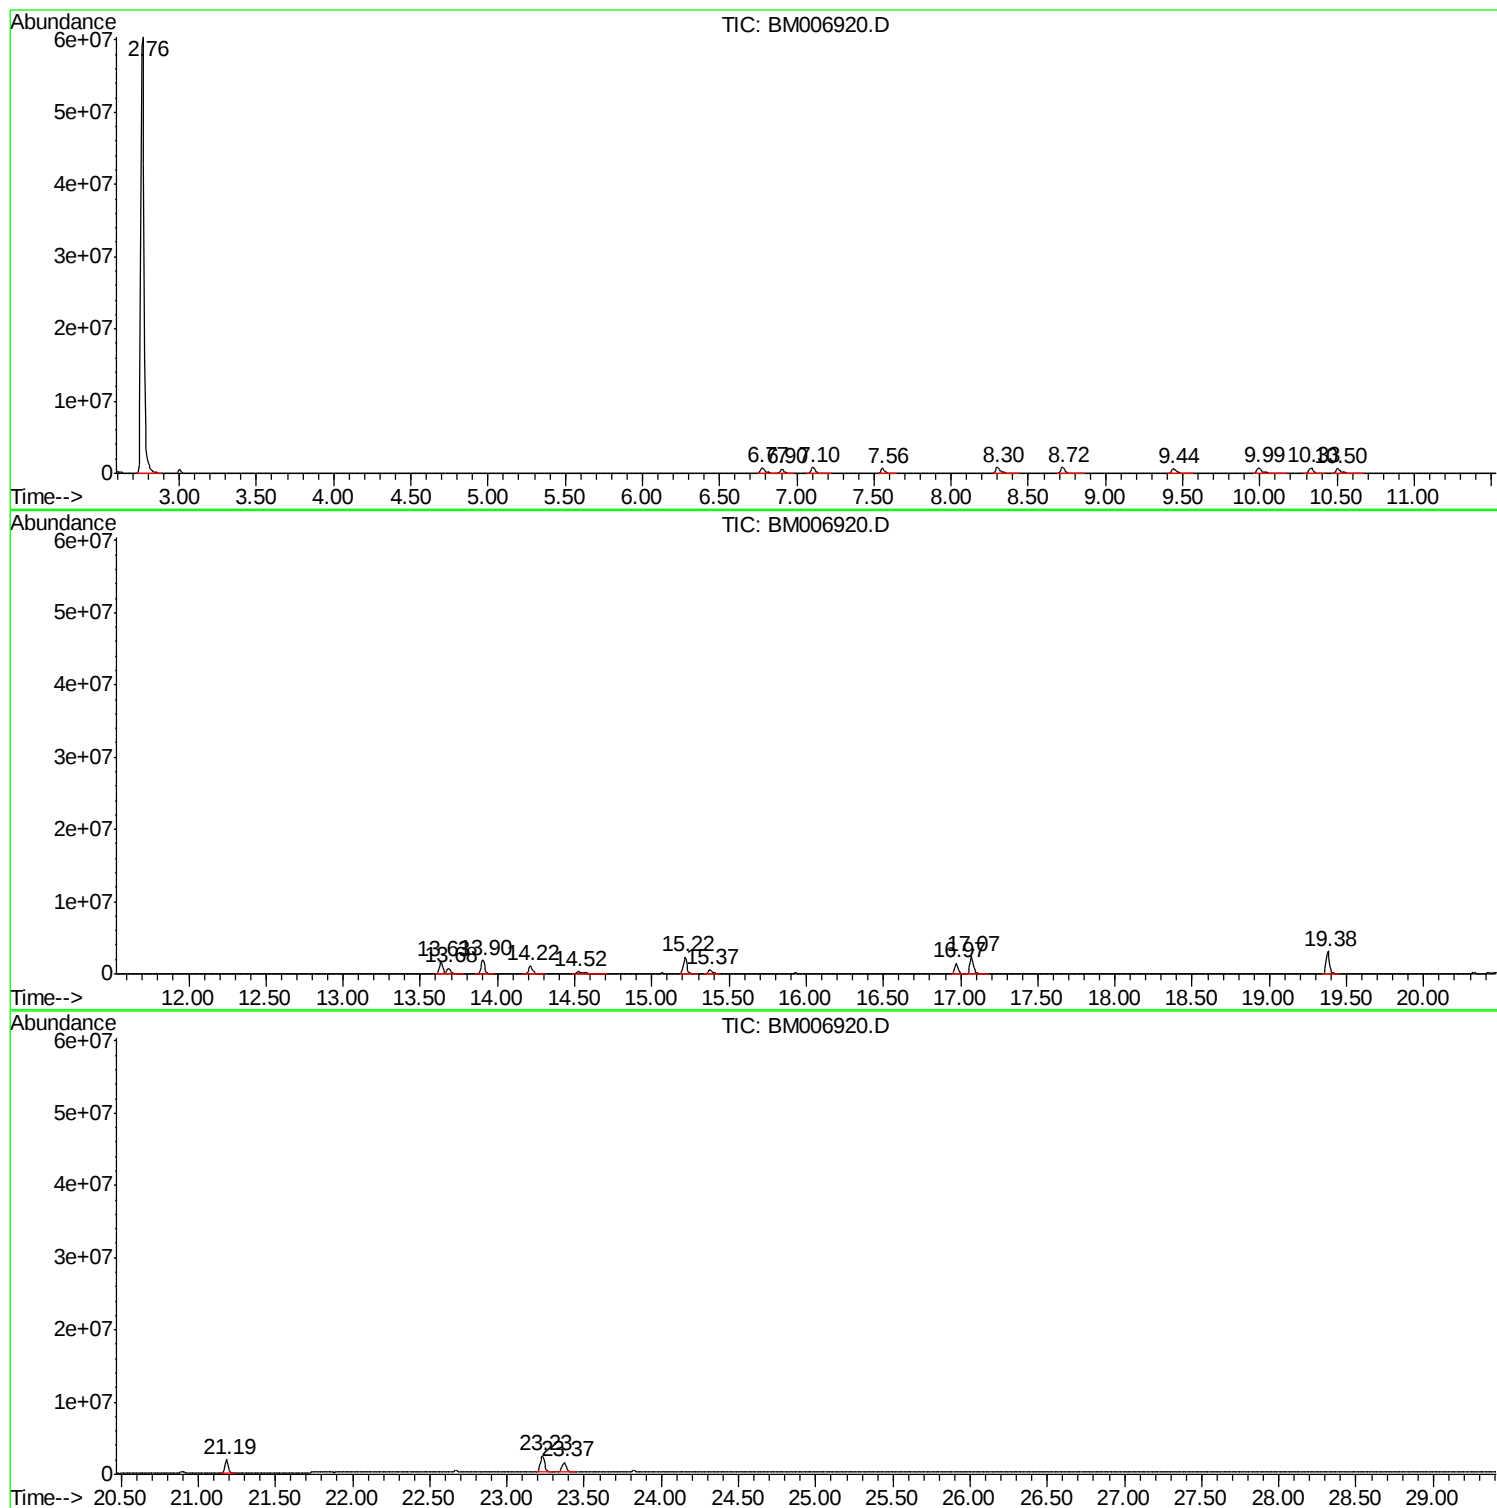

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006920.D
Acq On : 06 Aug 2016 03:20
Operator : UM/SJ
Sample : H4278-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJS0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006920.D
Acq On : 06 Aug 2016 03:20
Operator : UM/SJ
Sample : H4278-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJS0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc