

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006921.D
 Acq On : 06 Aug 2016 03:57
 Operator : UM/SJ
 Sample : H4278-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJS3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.763	25	30	42	rVB	214066	397005	10.51%	0.875%
2	4.746	362	367	372	rBV2	21801	42385	1.12%	0.093%
3	6.781	707	713	729	rBV	588122	1335304	35.34%	2.944%
4	6.904	729	734	749	rVB	491298	844054	22.34%	1.861%
5	7.104	762	768	784	rBV	686133	1294170	34.25%	2.854%
6	7.557	839	845	860	rBV	685733	1236988	32.74%	2.728%
7	8.304	966	972	989	rBV	654705	1461682	38.69%	3.223%
8	8.722	1036	1043	1064	rBV	664569	1358190	35.95%	2.995%
9	9.439	1159	1165	1188	rBV2	522509	1166138	30.87%	2.571%
10	9.992	1253	1259	1282	rBV2	583234	1520693	40.25%	3.353%
11	10.333	1308	1317	1336	rBV	867211	1631617	43.19%	3.598%
12	10.504	1340	1346	1375	rBV2	559557	1488927	39.41%	3.283%
13	13.633	1872	1878	1883	rBV	1494860	2210059	58.50%	4.873%
14	13.680	1883	1886	1900	rVB	679149	1113207	29.46%	2.455%
15	13.904	1917	1924	1941	rBV	1528885	2517892	66.64%	5.552%
16	14.215	1969	1977	1990	rBV2	1218088	2042413	54.06%	4.503%
17	14.527	2025	2030	2041	rBV3	224629	724772	19.18%	1.598%
18	15.062	2117	2121	2126	rBV3	30945	45274	1.20%	0.100%
19	15.215	2140	2147	2158	rBV	1965540	3095361	81.93%	6.825%
20	15.374	2169	2174	2185	rBV2	425802	838125	22.18%	1.848%
21	15.927	2264	2268	2271	rBV4	36582	54481	1.44%	0.120%
22	16.968	2439	2445	2456	rBV	1564127	2465970	65.27%	5.437%
23	17.068	2456	2462	2478	rVB2	2062254	3299823	87.34%	7.276%
24	17.874	2595	2599	2607	rBV9	23333	53485	1.42%	0.118%
25	19.380	2849	2855	2867	rBV	2493141	3778155	100.00%	8.331%
26	19.827	2927	2931	2938	rBV4	46922	70445	1.86%	0.155%
27	21.186	3156	3162	3172	rBV	2023222	2991463	79.18%	6.596%
28	23.227	3502	3509	3519	rBV2	1930703	3601498	95.32%	7.941%
29	23.368	3527	3533	3547	rVB	1338022	2672660	70.74%	5.893%


Sum of corrected areas: 45352236

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006921.D
Acq On : 06 Aug 2016 03:57
Operator : UM/SJ
Sample : H4278-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJS3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

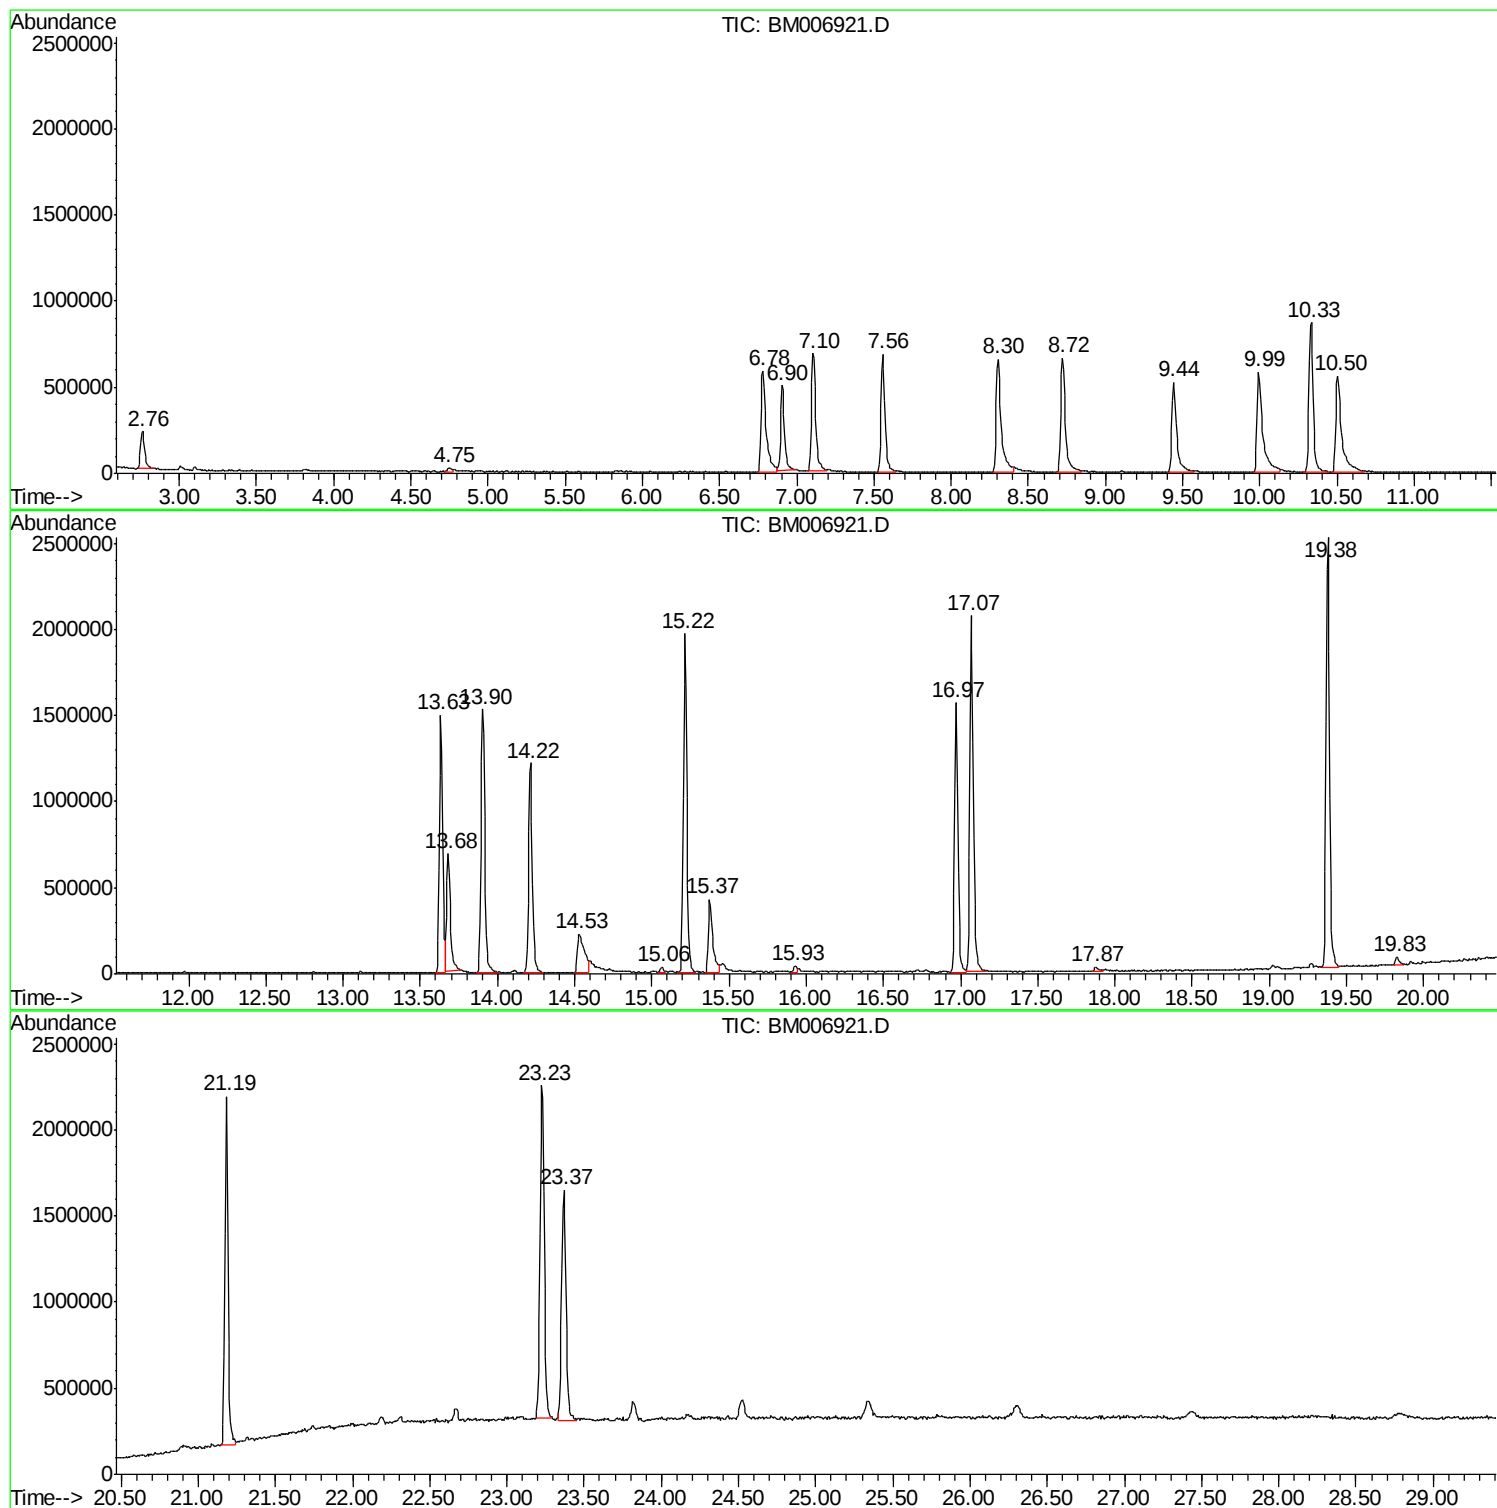

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006921.D
Acq On : 06 Aug 2016 03:57
Operator : UM/SJ
Sample : H4278-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJS3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006921.D
Acq On : 06 Aug 2016 03:57
Operator : UM/SJ
Sample : H4278-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJS3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc