

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
 Data File : BM006926.D
 Acq On : 06 Aug 2016 06:58
 Operator : UM/SJ
 Sample : H4278-15
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJS6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.640	5	9	15	rVB6	25043	41546	1.07%	0.091%
2	6.781	707	713	729	rBV	544255	1323096	34.16%	2.883%
3	6.904	729	734	748	rVB	490838	850263	21.95%	1.853%
4	7.104	762	768	783	rBV	692719	1283449	33.14%	2.797%
5	7.557	839	845	860	rBV	740464	1313801	33.92%	2.863%
6	8.298	966	971	993	rBV	645452	1496918	38.65%	3.262%
7	8.722	1037	1043	1064	rBV	678801	1355835	35.01%	2.955%
8	9.439	1159	1165	1186	rBV	548509	1186636	30.64%	2.586%
9	9.992	1253	1259	1285	rBV	593073	1567103	40.46%	3.415%
10	10.328	1310	1316	1339	rVB	946041	1787586	46.15%	3.896%
11	10.504	1339	1346	1370	rBV	596527	1537964	39.71%	3.352%
12	13.633	1872	1878	1882	rBV	1488059	2111846	54.53%	4.602%
13	13.680	1882	1886	1902	rVB	613933	1088602	28.11%	2.372%
14	13.904	1918	1924	1940	rBV	1557610	2495884	64.44%	5.439%
15	14.210	1970	1976	1991	rVV2	1352149	2209714	57.05%	4.815%
16	14.545	2027	2033	2042	rBV3	129822	423476	10.93%	0.923%
17	15.063	2117	2121	2127	rBV	52353	71955	1.86%	0.157%
18	15.216	2140	2147	2161	rBV	1950217	3072629	79.33%	6.696%
19	15.380	2170	2175	2185	rBV	245029	504680	13.03%	1.100%
20	15.451	2185	2187	2195	rVB6	45936	91968	2.37%	0.200%
21	15.927	2264	2268	2277	rBV2	59969	116727	3.01%	0.254%
22	16.968	2439	2445	2456	rBV	1695733	2636720	68.08%	5.746%
23	17.068	2456	2462	2480	rVB2	2162046	3357269	86.68%	7.316%
24	17.868	2595	2598	2605	rBV4	38734	74823	1.93%	0.163%
25	19.374	2849	2854	2869	rVB	2576447	3873042	100.00%	8.440%
26	20.880	3107	3110	3121	rBV4	82317	205863	5.32%	0.449%
27	21.180	3156	3161	3171	rBV	2307206	3184683	82.23%	6.940%
28	23.227	3502	3509	3520	rVB2	1973375	3741033	96.59%	8.152%
29	23.362	3526	3532	3545	rVB	1464778	2883373	74.45%	6.283%


Sum of corrected areas: 45888484

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006926.D
Acq On : 06 Aug 2016 06:58
Operator : UM/SJ
Sample : H4278-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJS6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

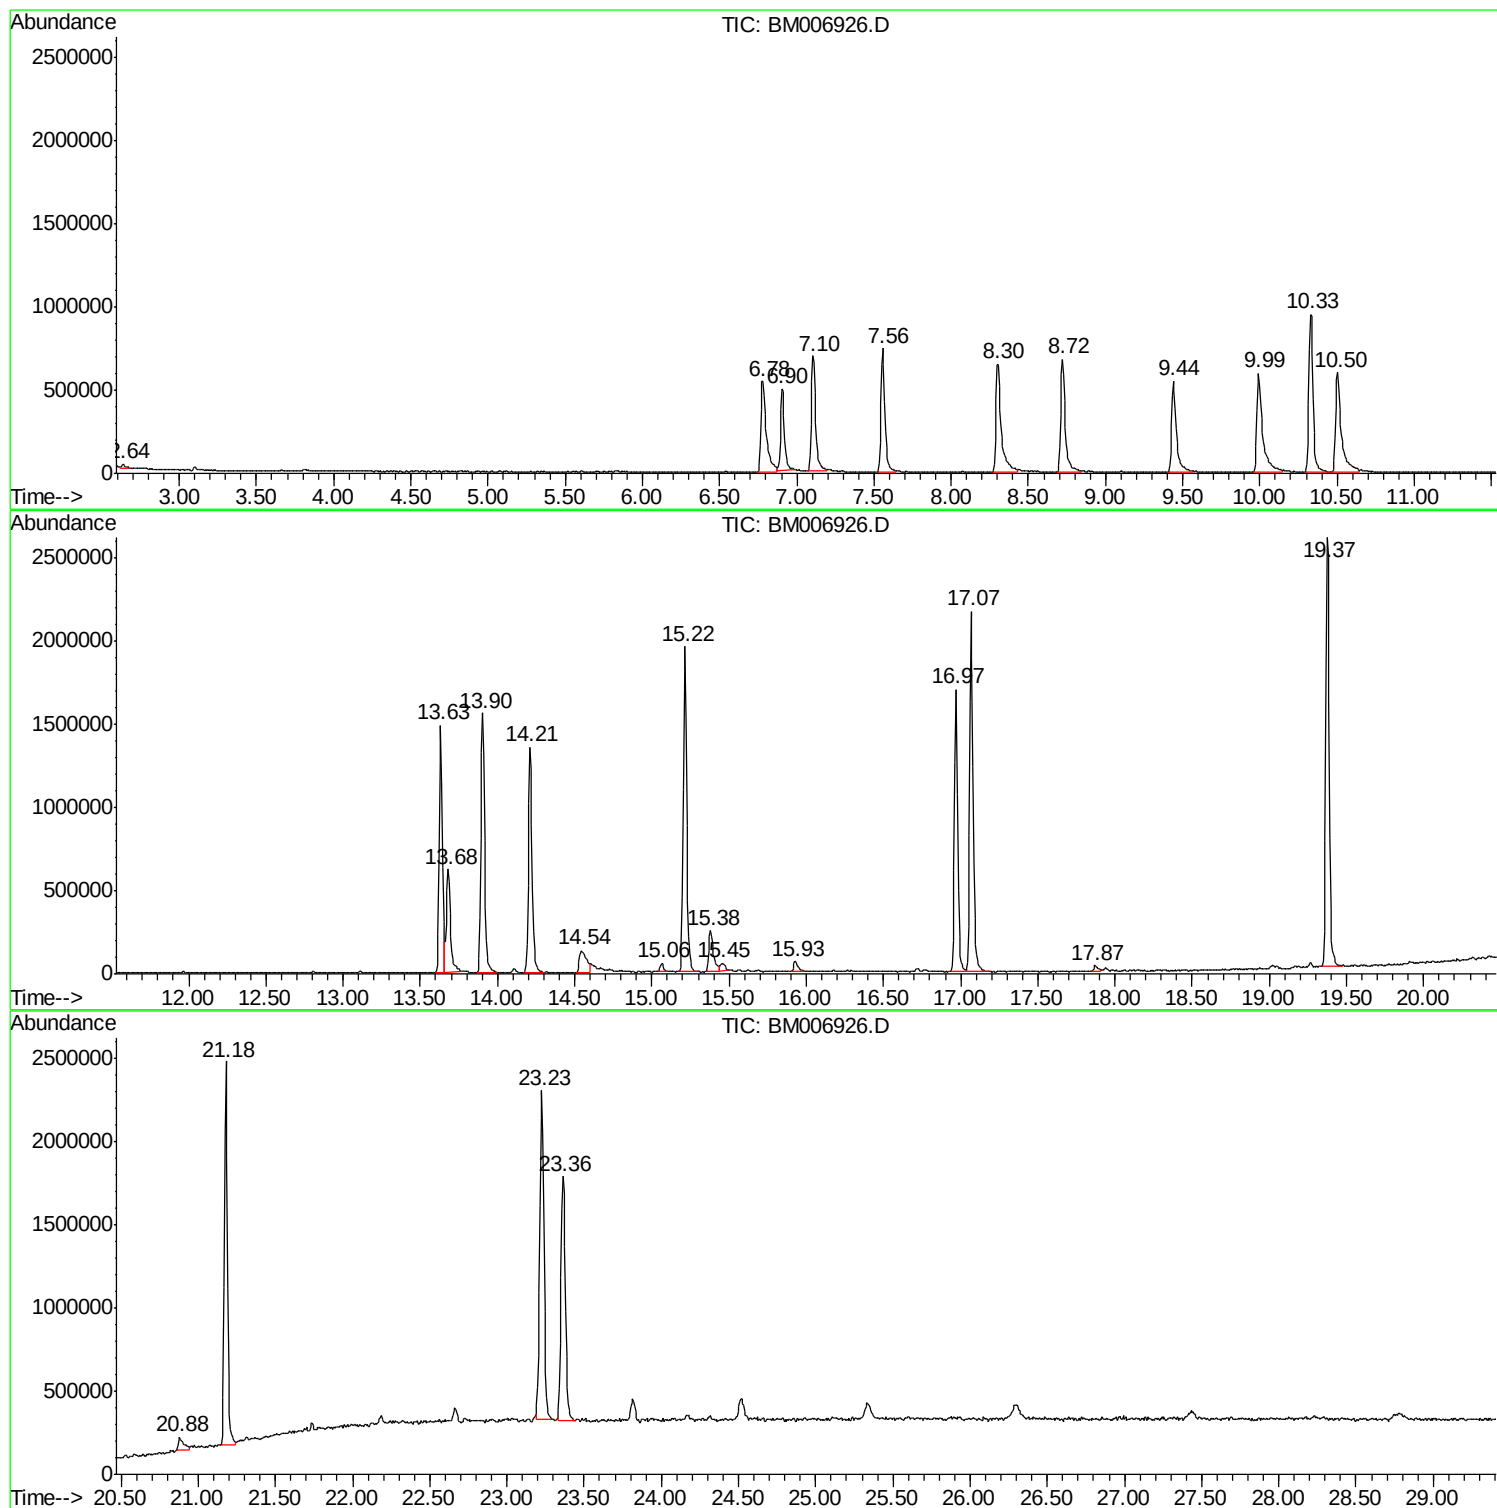

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006926.D
Acq On : 06 Aug 2016 06:58
Operator : UM/SJ
Sample : H4278-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJS6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080516\
Data File : BM006926.D
Acq On : 06 Aug 2016 06:58
Operator : UM/SJ
Sample : H4278-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJS6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc