


Data Path : Z:\HPCHEM1\BNA M\Data\BM080517\
 Data File : BM011137.D
 Acq On : 05 Aug 2017 10:51
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

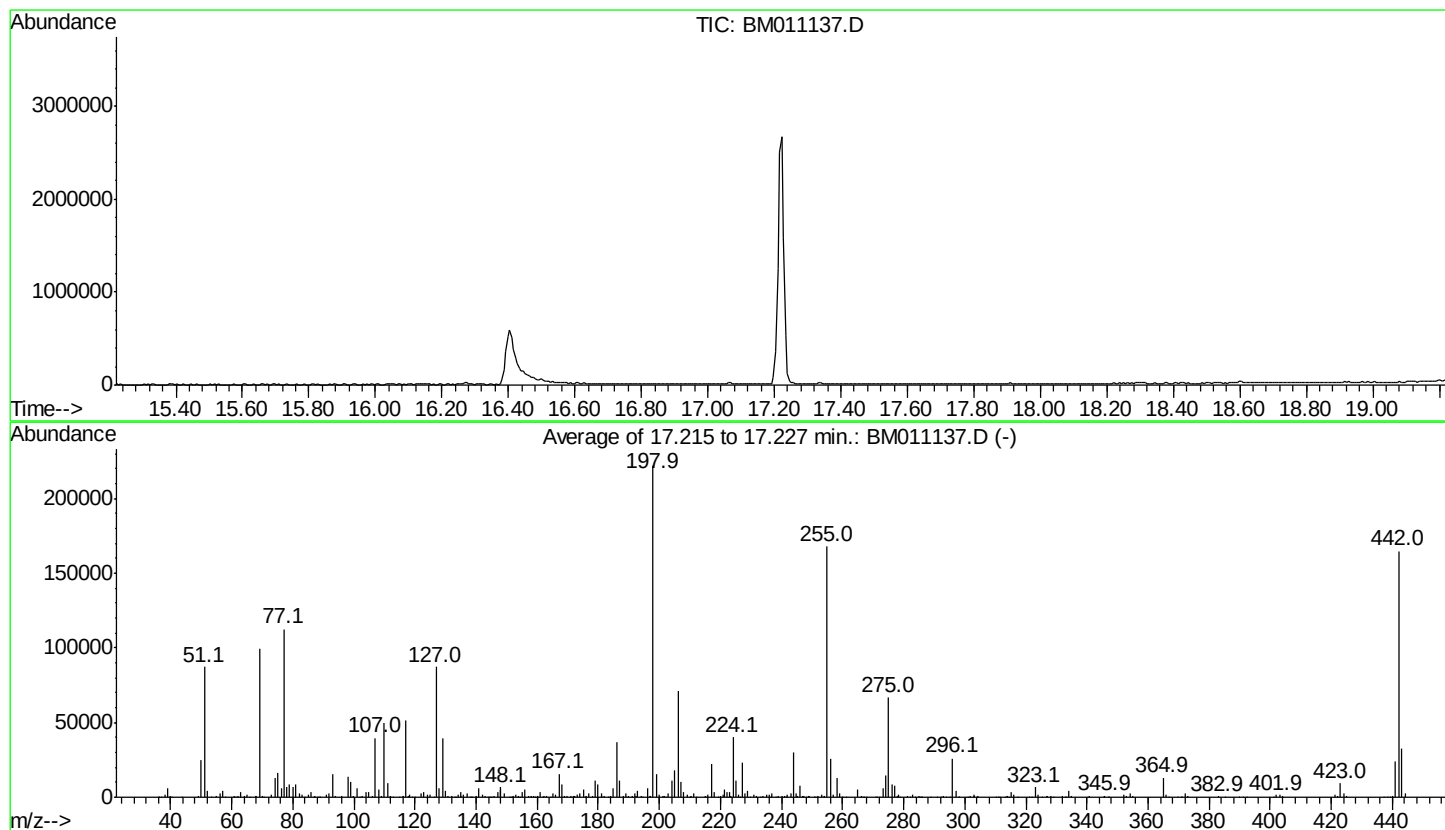

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	87112	PASS
68	69	0.00	2	1.1	1079	PASS
69	198	0.00	100	44.7	99112	PASS
70	69	0.00	2	0.8	778	PASS
127	198	10	80	39.3	87242	PASS
197	198	0.00	2	0.5	1205	PASS
198	198	100	100	100.0	221888	PASS
199	198	5	9	7.0	15583	PASS
275	198	10	60	30.1	66736	PASS
365	198	1	100	5.8	12870	PASS
441	443	0.01	100	74.6	24032	PASS
442	198	50	100	74.2	164586	PASS
443	442	15	24	19.6	32210	PASS