
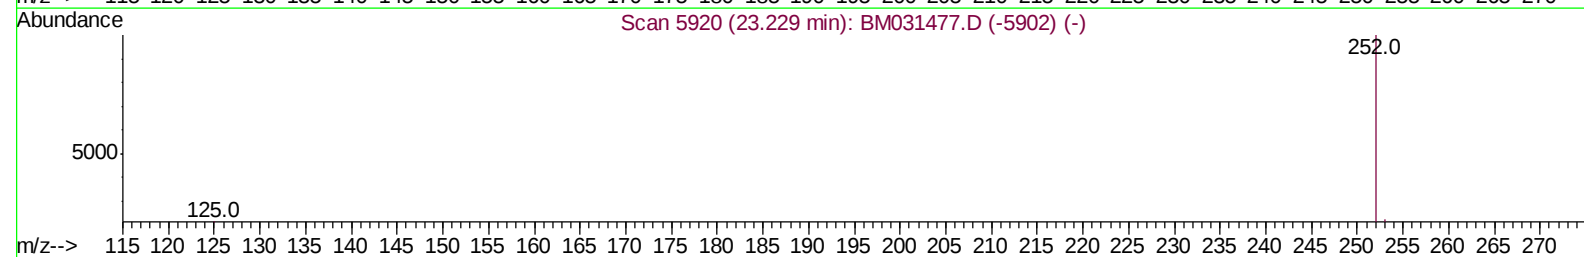
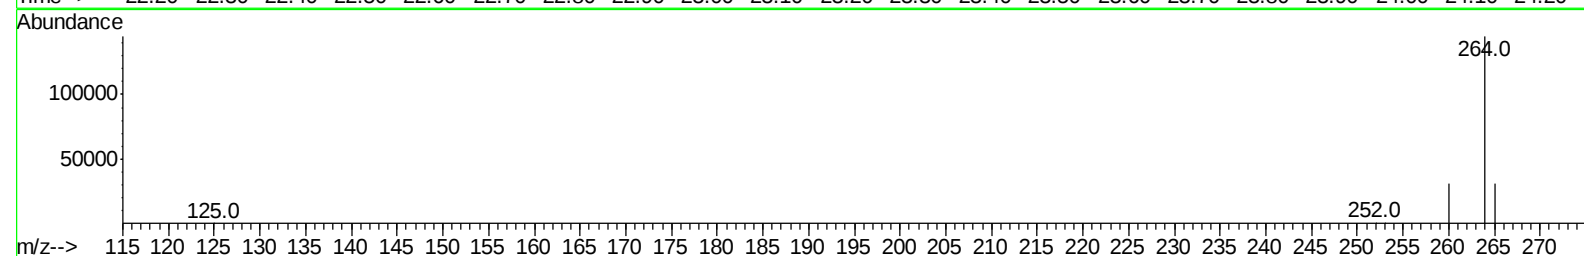


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080521\
Data File : BM031480.D
Acq On : 05 Aug 2021 12:39
Operator : CG/JU
Sample : M3141-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 05 13:10:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 05 11:03:39 2021
Response via : Initial Calibration

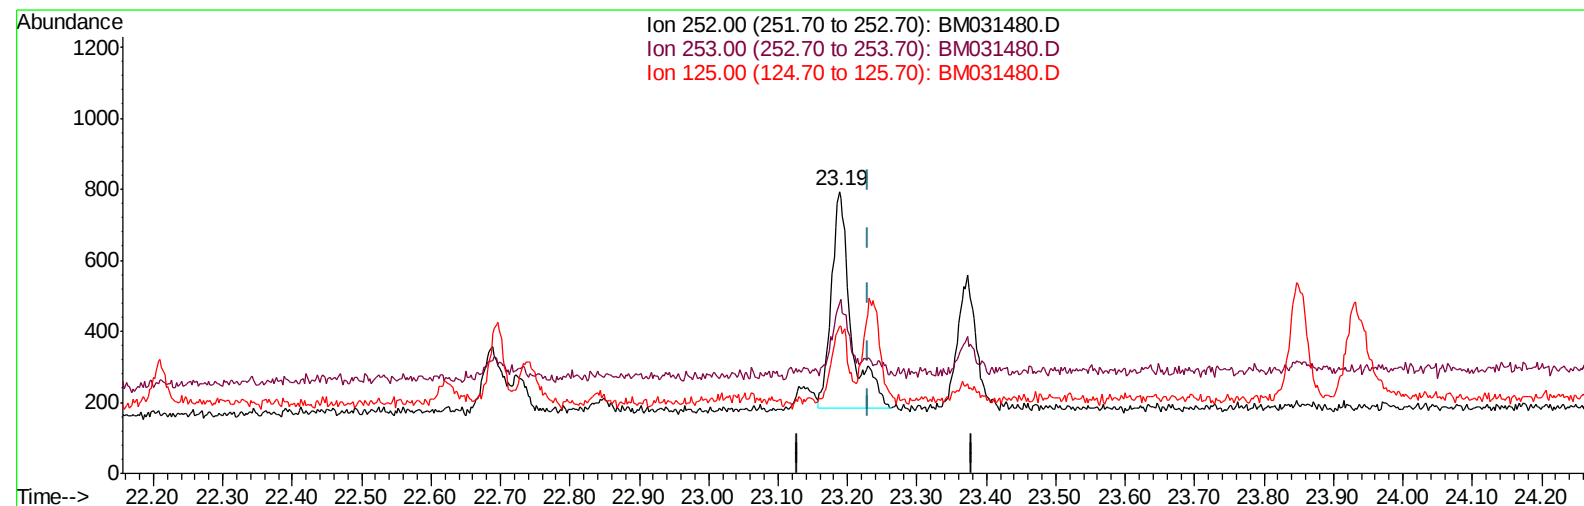

TIC: BM031480.D

(26) Benzo(a)pyrene (C)
23.188min (-0.041) 0.09ng/ul
response 1183

Ion	Exp%	Act%
252.00	100	100
253.00	28.00	60.28#
125.00	16.20	52.08#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080521\
 Data File : BM031480.D
 Acq On : 05 Aug 2021 12:39
 Operator : CG/JU
 Sample : M3141-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 05 13:13:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 05 11:03:39 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	751	0.40	ng/ul	0.00
4) Naphthalene-d8	10.35	136	2996	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.22	164	2003	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.97	188	4030	0.40	ng/ul	0.00
17) Chrysene-d12	21.17	240	3221	0.40	ng/ul	0.00
23) Perylene-d12	23.32	264	3369	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.19	96	2258	2.71	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.95	152	1113	0.22	ng/ul	0.00
18) Fluoranthene-d10	19.00	212	3997	0.37	ng/ul	0.00
Target Compounds				Ovalue		
19) Fluoranthene	19.04	202	441	0.032	ng/ul#	54
20) Pyrene	19.39	202	381	0.027	ng/ul#	28
22) Chrysene	21.20	228	273	0.020	ng/ul#	68
24) Benzo(b)fluoranthene	22.69	252	402	0.026	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080521\
Data File : BM031480.D
Acq On : 05 Aug 2021 12:39
Operator : CG/JU
Sample : M3141-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 05 13:13:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 05 11:03:39 2021
Response via : Initial Calibration

