
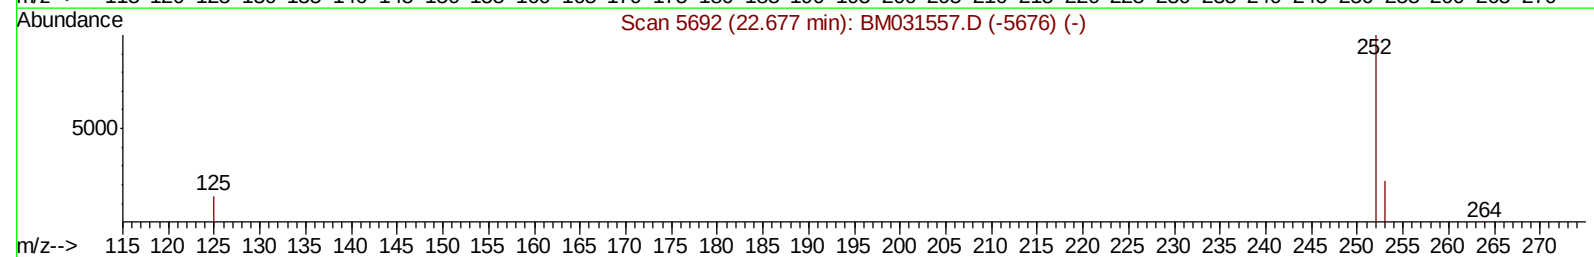
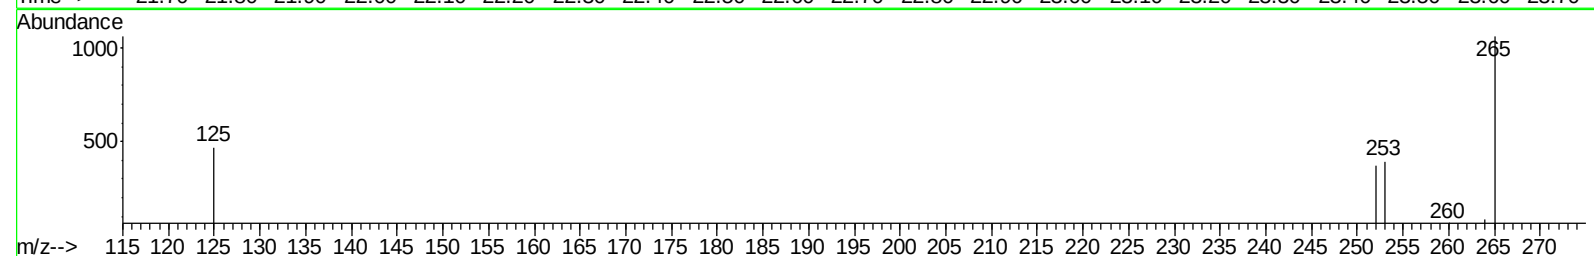


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080521\
 Data File : BM031572.D
 Acq On : 08 Aug 2021 04:25
 Operator : CG/JU
 Sample : M3163-16
 Misc :
 ALS Vial : 98 Sample Multiplier: 1

Quant Time: Aug 09 05:27:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 06 18:39:21 2021
 Response via : Initial Calibration

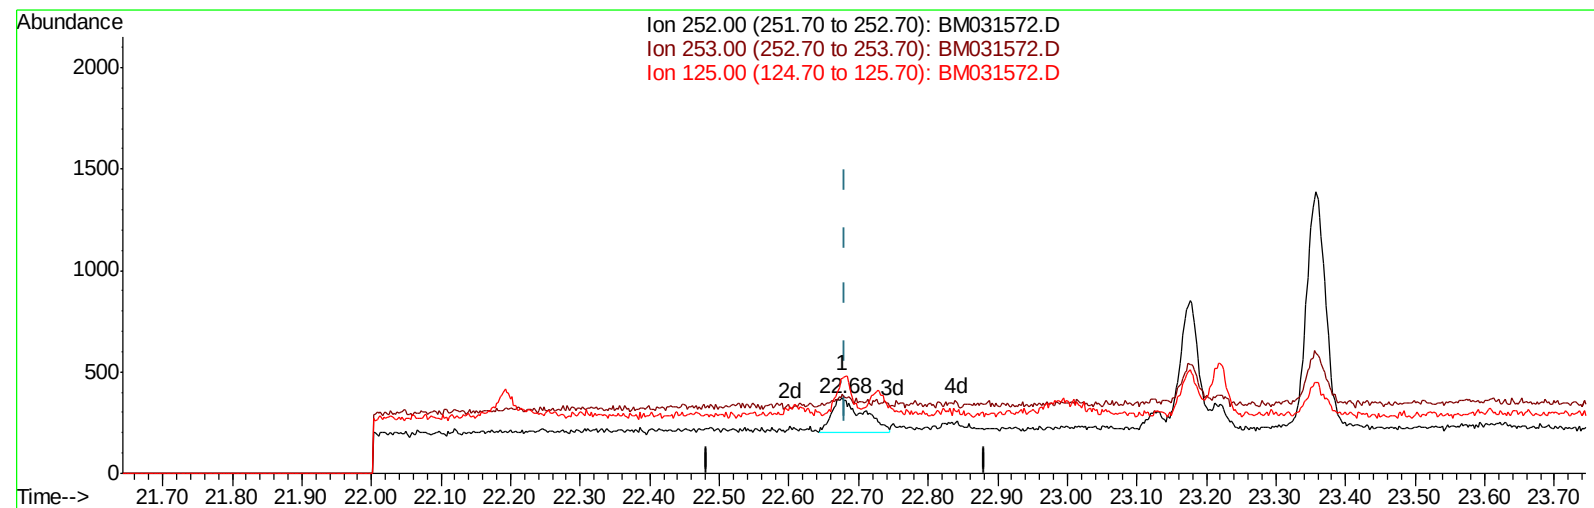

TIC: BM031572.D

(24) Benzo(b)fluoranthene




22.677min (-0.005) 0.03ng/ul

response 523

Ion	Exp%	Act%
252.00	100	100
253.00	26.50	105.91#
125.00	11.40	126.08#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080521\
 Data File : BM031572.D
 Acq On : 08 Aug 2021 04:25
 Operator : CG/JU
 Sample : M3163-16
 Misc :
 ALS Vial : 98 Sample Multiplier: 1

Quant Time: Aug 09 05:27:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 06 18:39:21 2021
 Response via : Initial Calibration

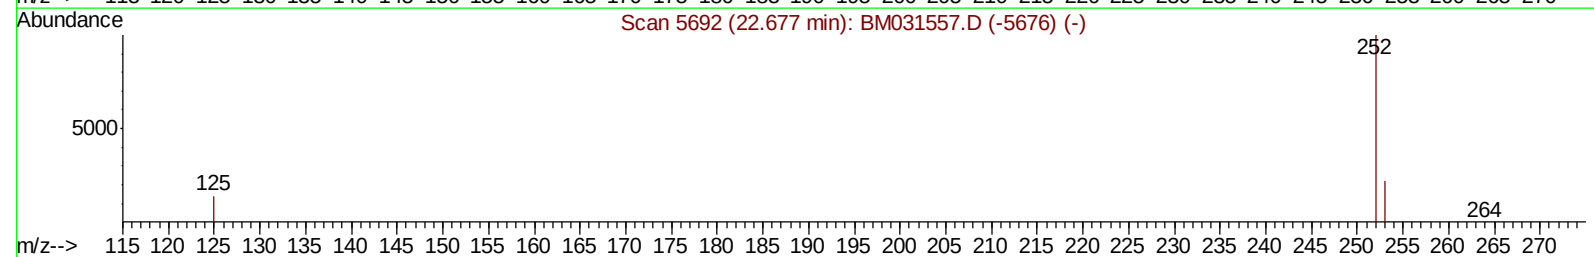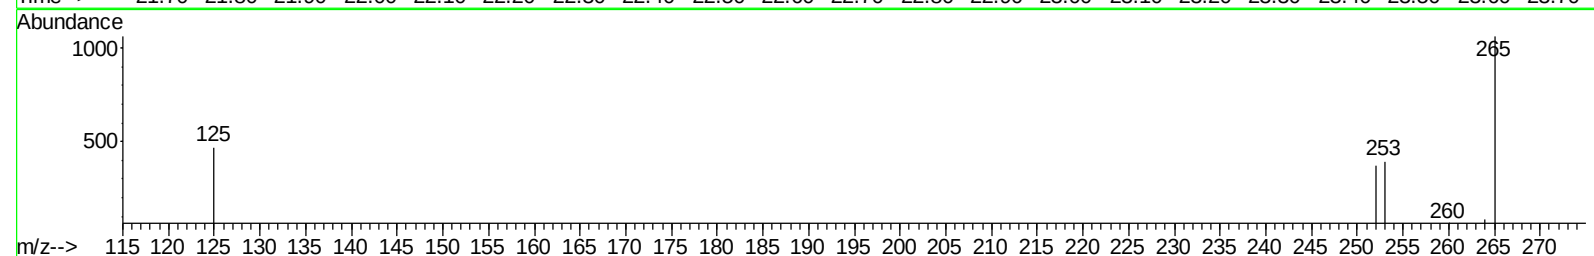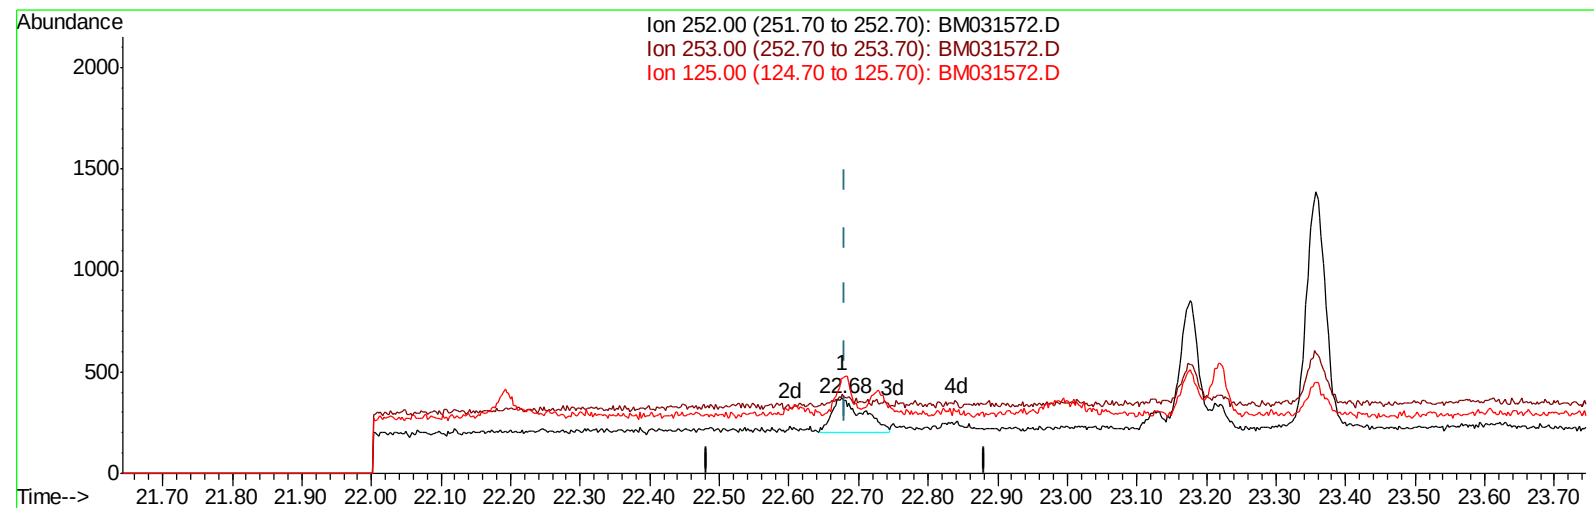

TIC: BM031572.D

(24) Benzo(b)fluoranthene

22.677min (-0.005) 0.03ng/ul

response 523

Ion	Exp%	Act%
252.00	100	100
253.00	26.50	105.91#
125.00	11.40	126.08#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080521\
 Data File : BM031572.D
 Acq On : 08 Aug 2021 04:25
 Operator : CG/JU
 Sample : M3163-16
 Misc :
 ALS Vial : 98 Sample Multiplier: 1

Quant Time: Aug 09 05:33:47 2021

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072821.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Aug 06 18:39:21 2021

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	1244	0.40	ng/ul	0.00
4) Naphthalene-d8	10.34	136	4647	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.21	164	2720	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.96	188	5033	0.40	ng/ul	0.00
17) Chrysene-d12	21.16	240	3874	0.40	ng/ul	0.00
23) Perylene-d12	23.31	264	3999	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.19	96	6034	4.37	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.94	152	2313	0.30	ng/ul	0.00
18) Fluoranthene-d10	19.00	212	4349	0.34	ng/ul	0.00
Target Compounds						
					Ovalue	
19) Fluoranthene	19.03	202	464	0.028	ng/ul#	56
20) Pyrene	19.39	202	383	0.023	ng/ul#	43

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080521\
Data File : BM031572.D
Acq On : 08 Aug 2021 04:25
Operator : CG/JU
Sample : M3163-16
Misc :
ALS Vial : 98 Sample Multiplier: 1

Quant Time: Aug 09 05:33:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 06 18:39:21 2021
Response via : Initial Calibration

