

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080521\
 Data File : BM031516.D
 Acq On : 06 Aug 2021 15:17
 Operator : CG/JU
 Sample : M3162-08
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGET8

Quant Time: Aug 06 15:48:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 05 11:03:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	1304	0.400	ng/ul	0.00
4) Naphthalene-d8	10.347	136	4852	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.216	164	3067	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.964	188	5826	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.164	240	4572	0.400	ng/ul	0.00
23) Perylene-d12	23.316	264	4948	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.189	96	8841	6.105	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.944	152	3494	0.427	ng/ul	0.00
18) Fluoranthene-d10	19.001	212	7092	0.465	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.621	266	38	0.020	ng/ul#	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080521\
Data File : BM031516.D
Acq On : 06 Aug 2021 15:17
Operator : CG/JU
Sample : M3162-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGET8

Quant Time: Aug 06 15:48:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 05 11:03:39 2021
Response via : Initial Calibration

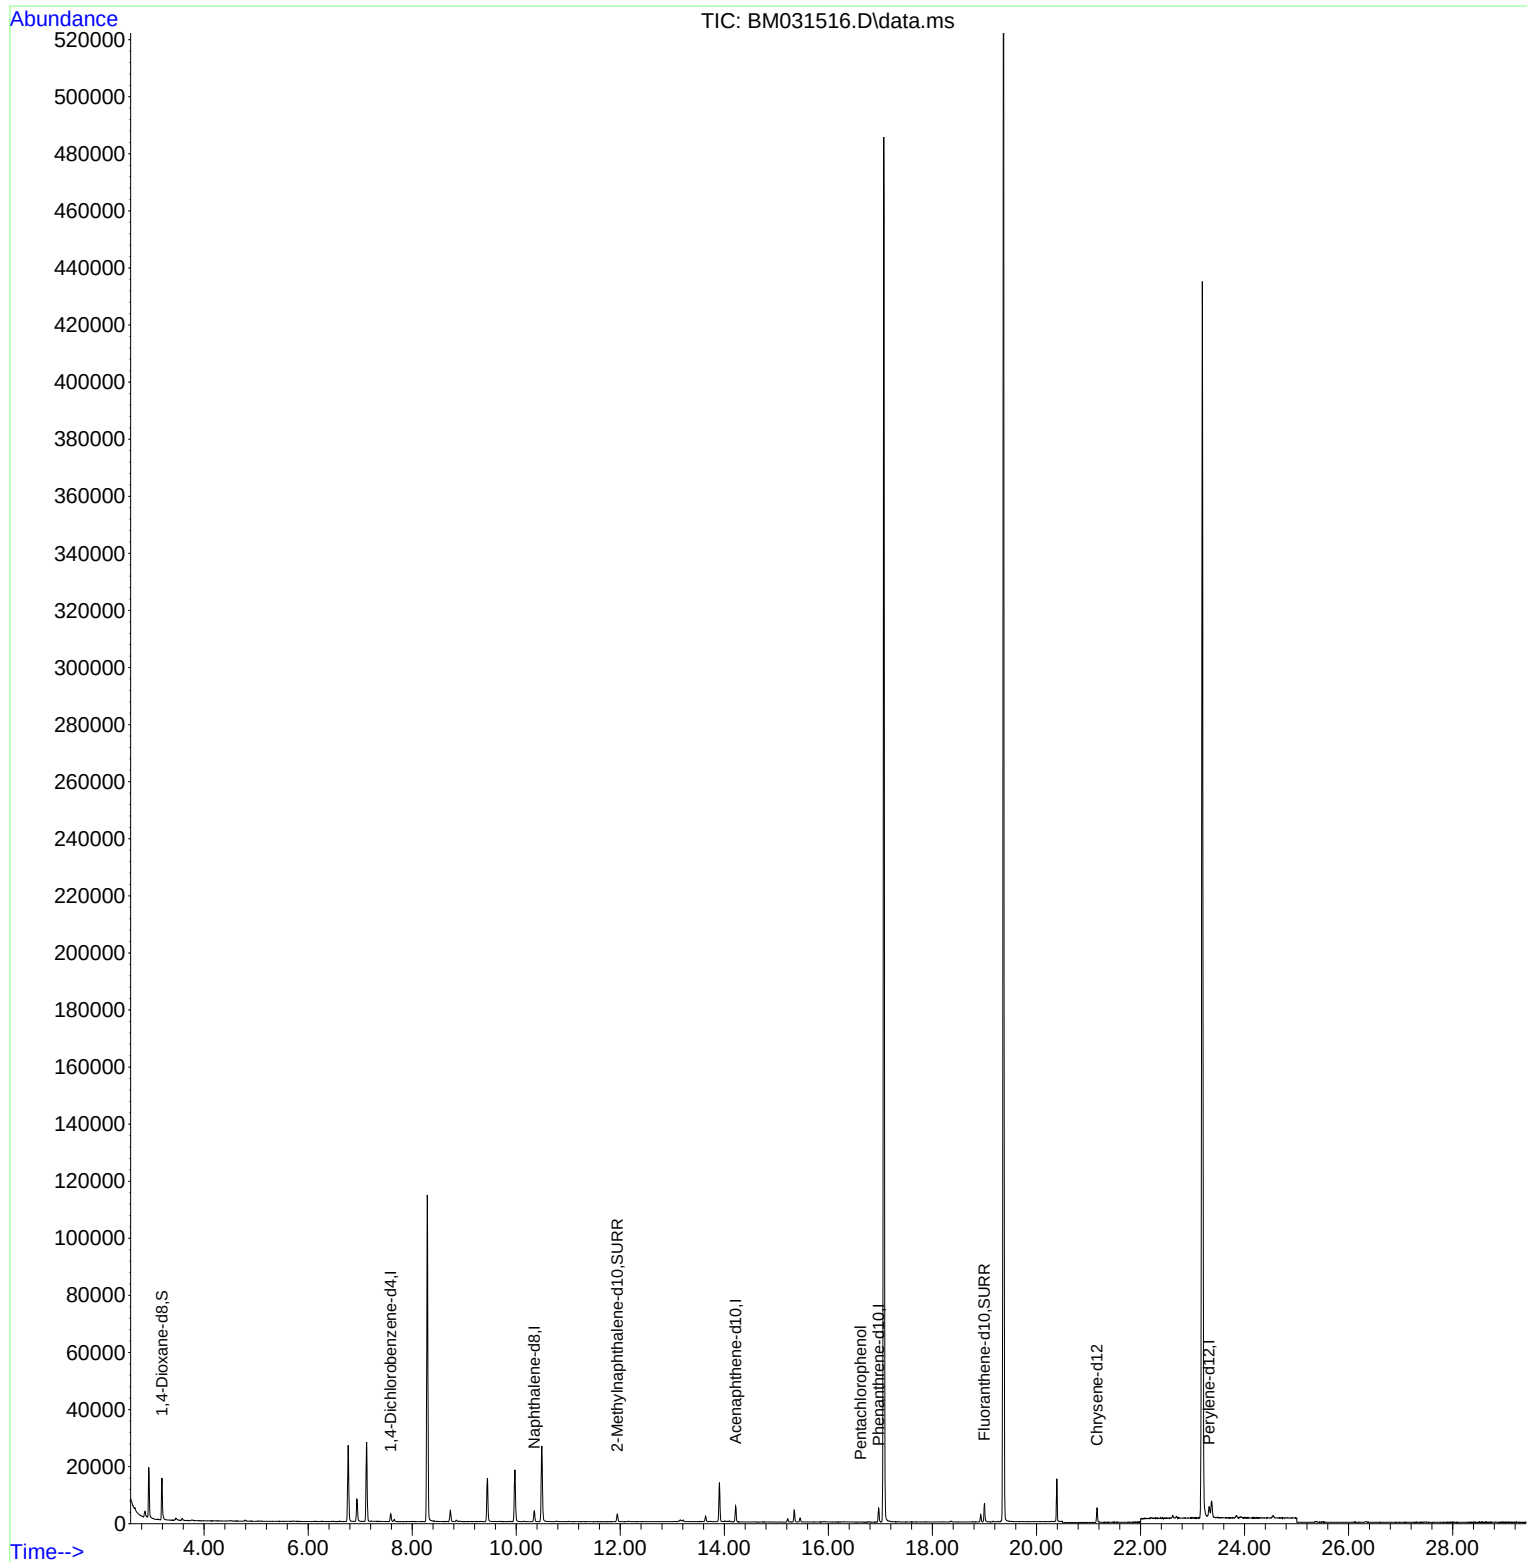

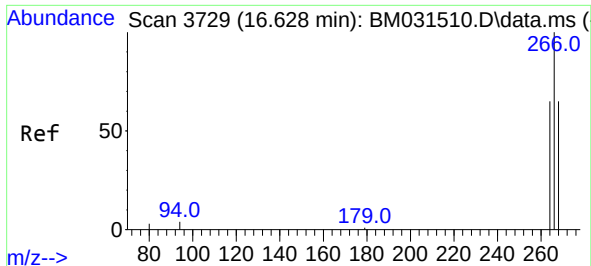

#14
 Pentachlorophenol
 Concen: 0.020 ng/ul
 RT: 16.621 min Scan# 3727
 Delta R.T. -0.010 min
 Lab File: BM031516.D
 Acq: 06 Aug 2021 15:17

Instrument :
 BNA_M
 ClientSampleId :
 BGET8

Tgt Ion:266 Resp: 38
 Ion Ratio Lower Upper
 266 100
 264 44.7 50.1 75.1#
 268 57.9 51.3 76.9

