

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080521\
 Data File : BM031572.D
 Acq On : 08 Aug 2021 04:25
 Operator : CG/JU
 Sample : M3163-16
 Misc :
 ALS Vial : 98 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGEZ5

Quant Time: Aug 09 04:12:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 06 18:39:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.580	152	1244	0.400	ng/ul	0.00
4) Naphthalene-d8	10.343	136	4647	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.212	164	2720	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.964	188	5033	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.159	240	3874	0.400	ng/ul	# 0.00
23) Perylene-d12	23.314	264	3999	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.185	96	6034	4.367	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.939	152	2313	0.295	ng/ul	0.00
18) Fluoranthene-d10	18.997	212	4349	0.336	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.027	202	464	0.028	ng/ul#	56
20) Pyrene	19.390	202	383	0.023	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080521\
Data File : BM031572.D
Acq On : 08 Aug 2021 04:25
Operator : CG/JU
Sample : M3163-16
Misc :
ALS Vial : 98 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGEZ5

Quant Time: Aug 09 04:12:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 06 18:39:21 2021
Response via : Initial Calibration




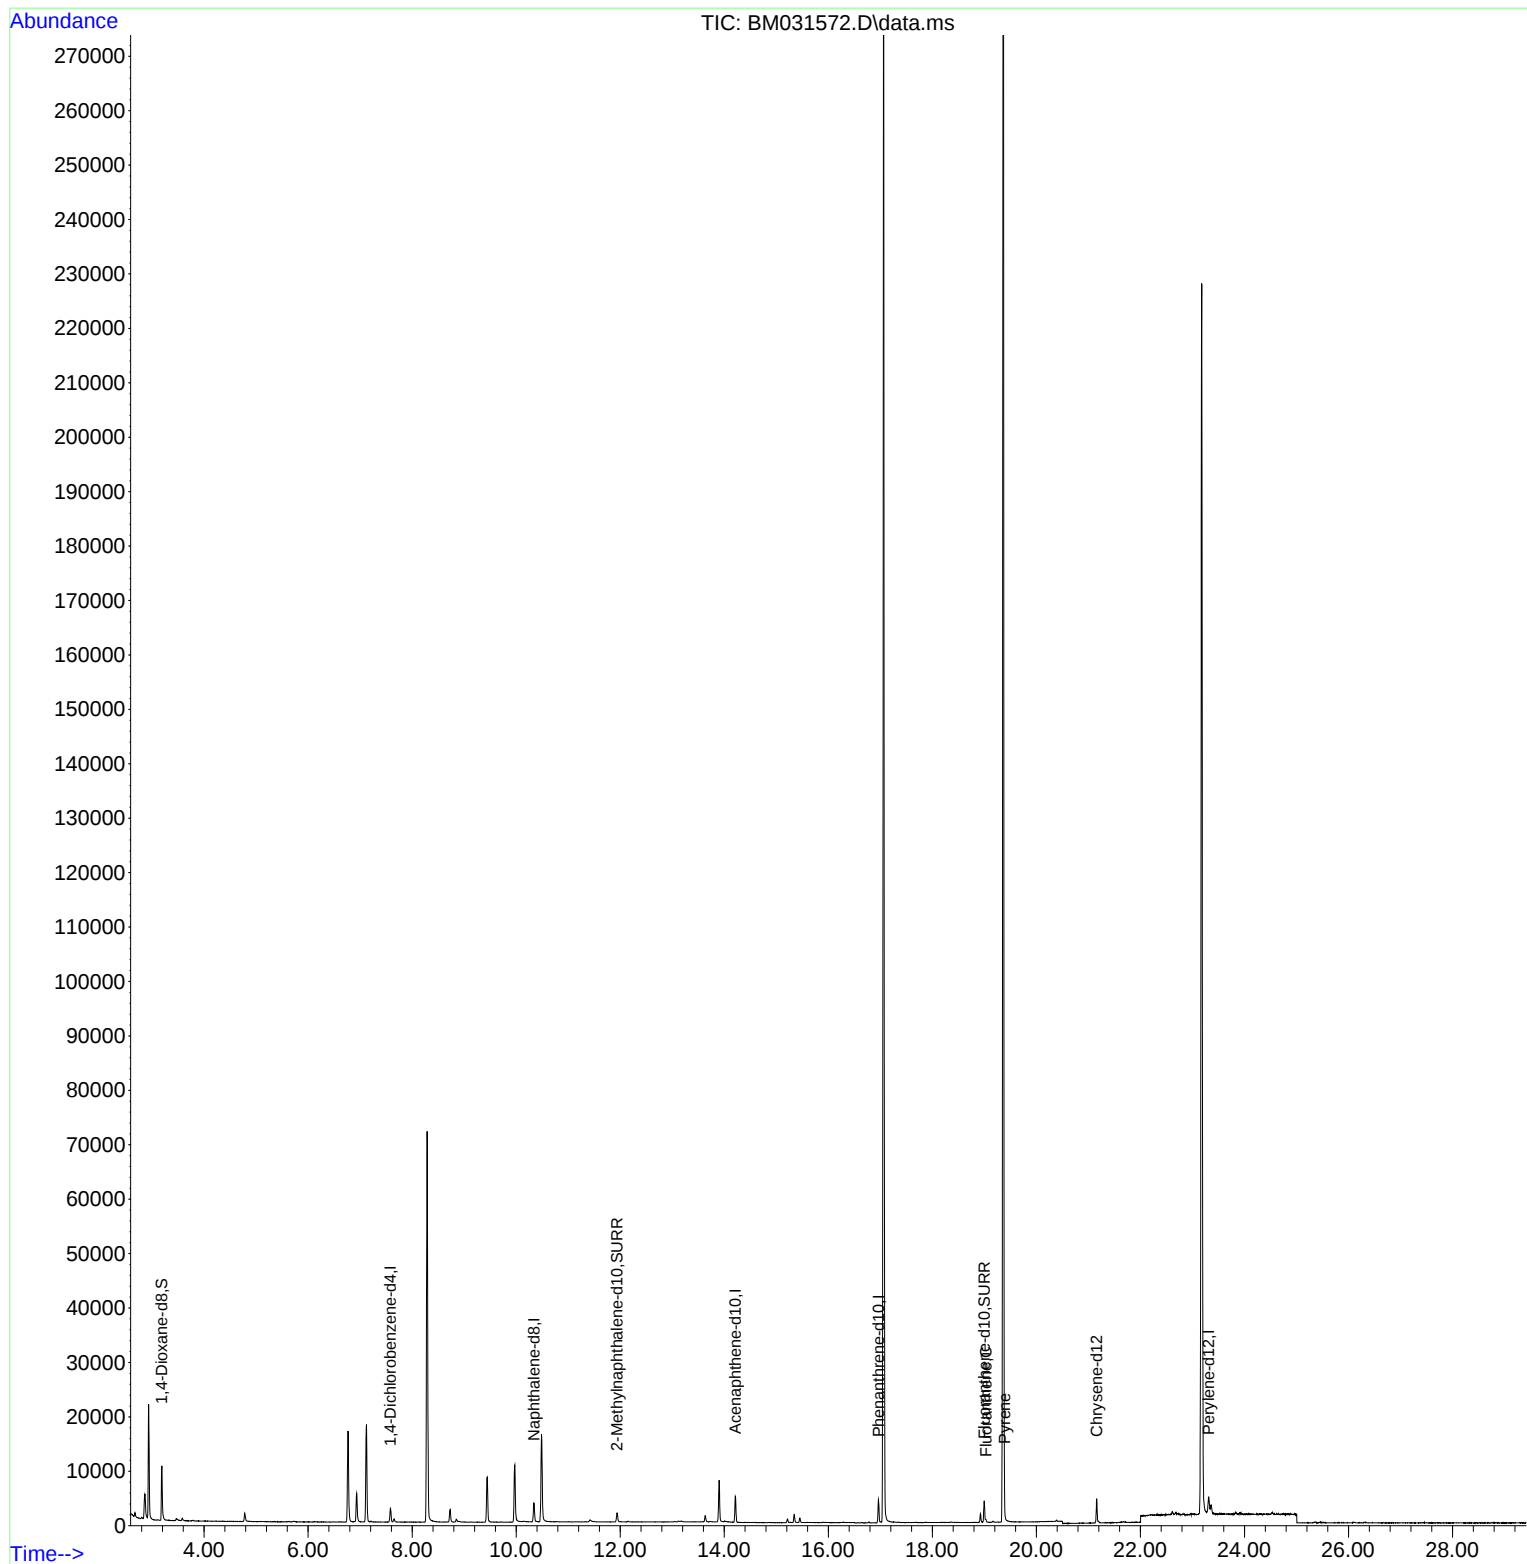


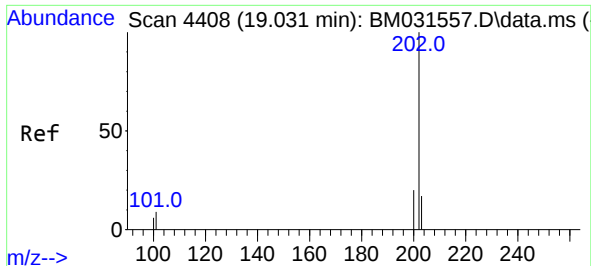

#19
Fluoranthene
Concen: 0.028 ng/ul
RT: 19.027 min Scan# 4407
Delta R.T. -0.004 min
Lab File: BM031572.D
Acq: 08 Aug 2021 04:25

Instrument :
BNA_M
ClientSampleId :
BGEZ5

Tgt Ion:202	Resp:	464
Ion Ratio	Lower	Upper
202	100	
101	24.7	6.6 10.0#
100	20.8	5.4 8.0#

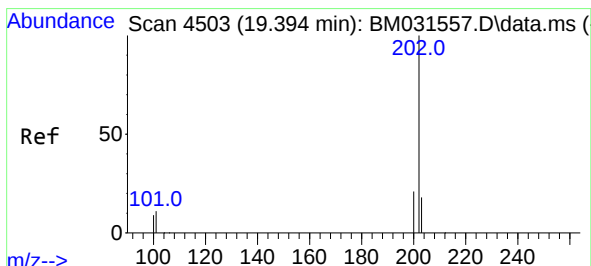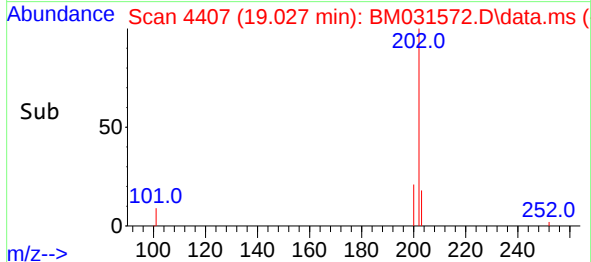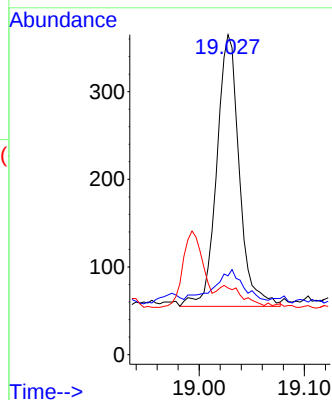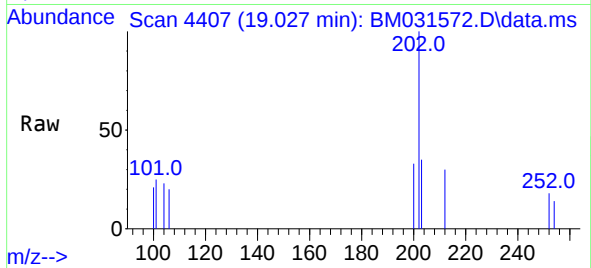

#20
Pyrene
Concen: 0.023 ng/ul
RT: 19.390 min Scan# 4502
Delta R.T. -0.008 min
Lab File: BM031572.D
Acq: 08 Aug 2021 04:25

Tgt Ion:202	Resp:	383
Ion Ratio	Lower	Upper
202	100	
101	26.7	7.8 11.6#
100	33.2	6.6 10.0#

