

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080624\
 Data File : BM047056.D
 Acq On : 07 Aug 2024 14:02
 Operator : RC/JU
 Sample : P3378-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AZ7

Quant Time: Aug 07 14:57:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 07 04:48:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.392	152	295696	20.000	ng/u1	0.00
20) Naphthalene-d8	10.151	136	1180699	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.051	164	746474	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.809	188	1551009	20.000	ng/u1	0.00
79) Chrysene-d12	21.044	240	1406575	20.000	ng/u1	0.00
88) Perylene-d12	23.750	264	1625062	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.022	96	26945	3.610	ng/uL	0.00
4) Pyridine-d5	3.410	84	181595	8.920	ng/u1	0.00
7) Phenol-d5	6.598	99	257623	11.469	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.751	67	353306	23.905	ng/u1	0.00
11) 2-Chlorophenol-d4	6.934	132	443741	23.321	ng/u1	0.00
15) 4-Methylphenol-d8	8.116	113	398316	22.384	ng/u1	0.00
21) Nitrobenzene-d5	8.539	128	221129	23.340	ng/u1	0.00
24) 2-Nitrophenol-d4	9.251	143	249485	24.113	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.786	165	472388	23.780	ng/u1	0.00
31) 4-Chloroaniline-d4	10.298	131	553898	21.216	ng/u1	0.00
46) Dimethylphthalate-d6	13.474	166	1352368	23.694	ng/u1	0.00
49) Acenaphthylene-d8	13.739	160	1546894	24.280	ng/u1	0.00
54) 4-Nitrophenol-d4	14.292	143	55636	5.041	ng/u1	0.00
60) Fluorene-d10	15.051	176	1146760	23.487	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.192	200	194687	19.868	ng/u1	0.00
73) Anthracene-d10	16.909	188	1719320	23.383	ng/u1	0.00
81) Pyrene-d10	19.221	212	1937745	24.066	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.568	264	2054978	24.015	ng/u1	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.198	128	253123	4.049	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080624\
Data File : BM047056.D
Acq On : 07 Aug 2024 14:02
Operator : RC/JU
Sample : P3378-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AZ7

Quant Time: Aug 07 14:57:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 07 04:48:25 2024
Response via : Initial Calibration

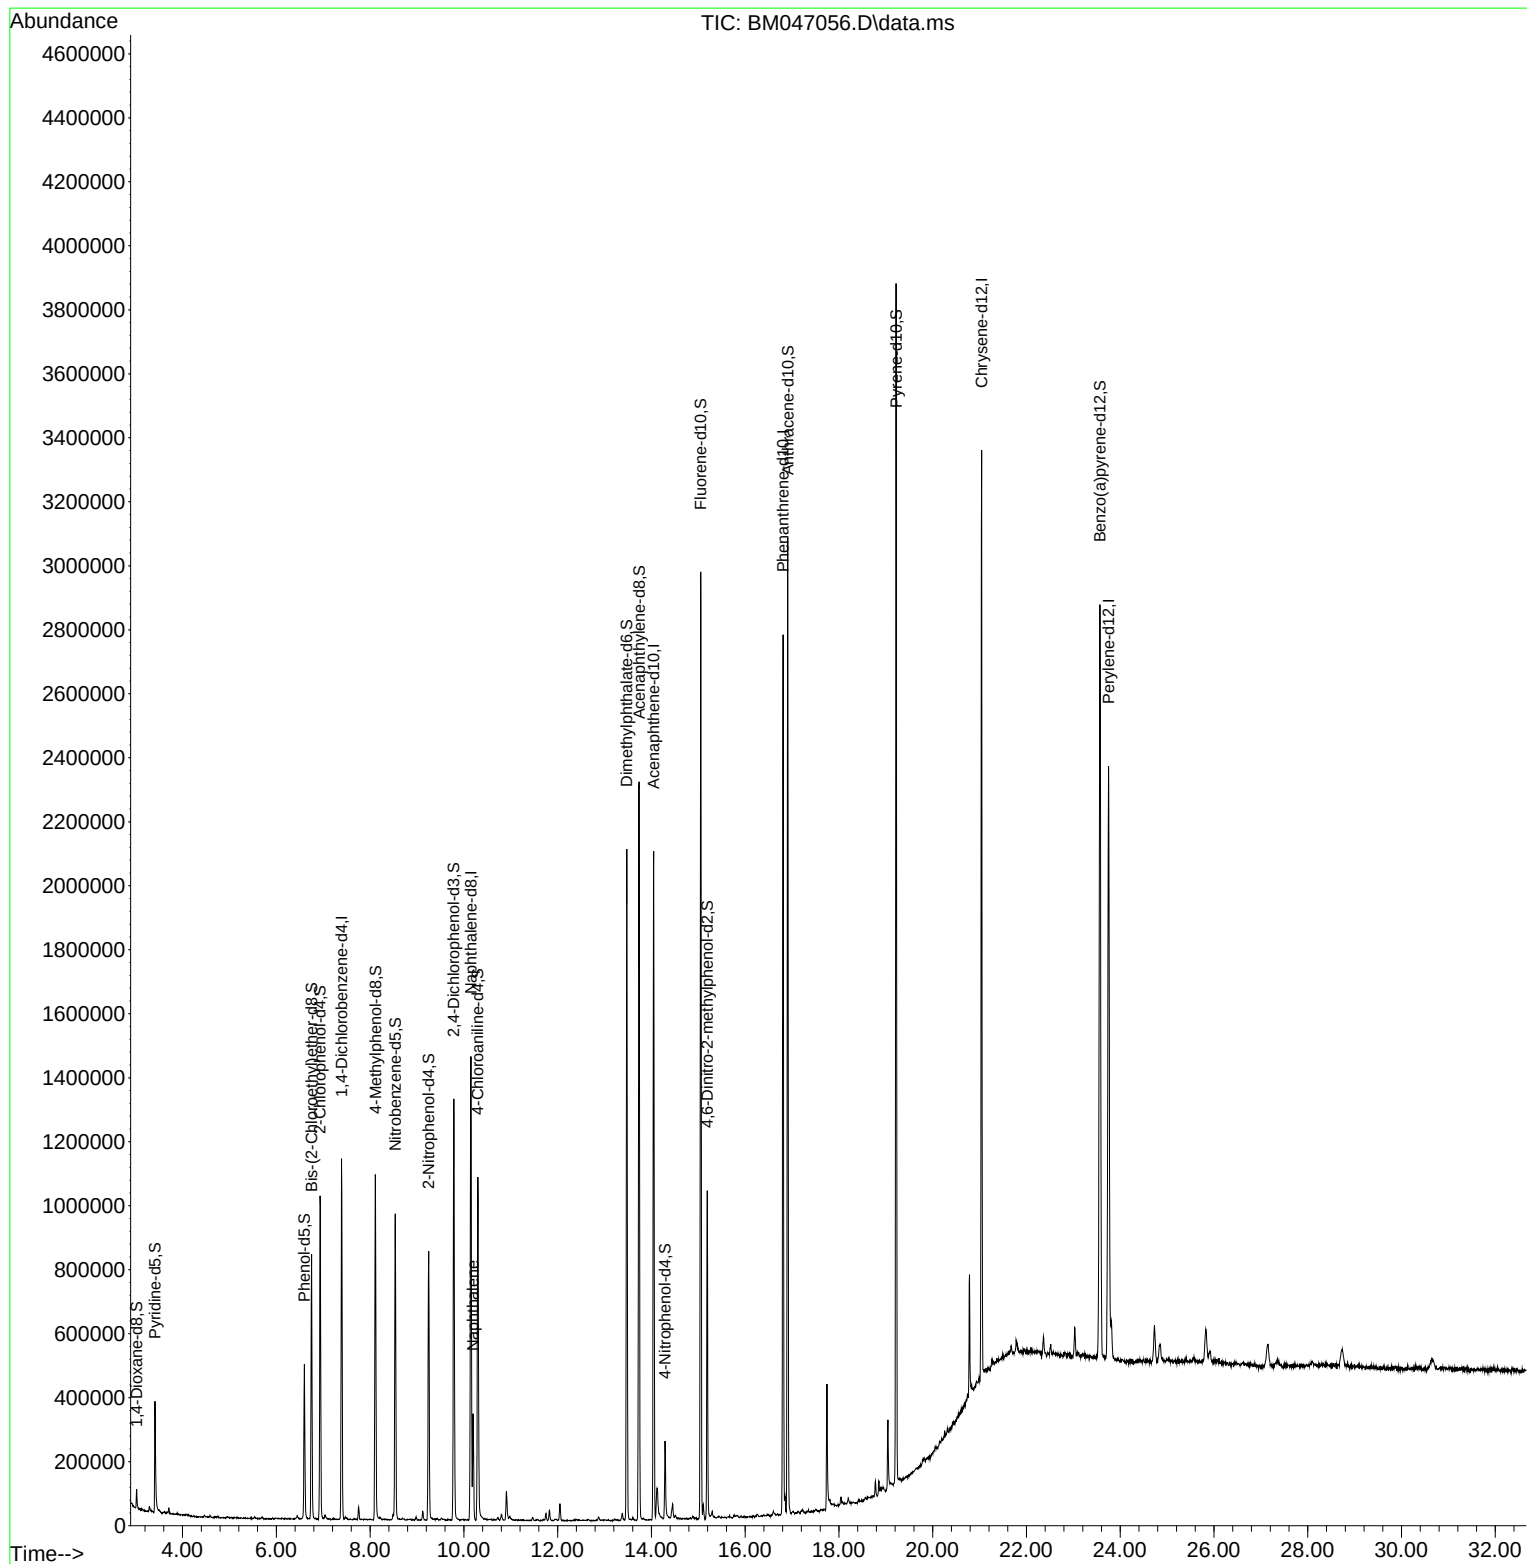

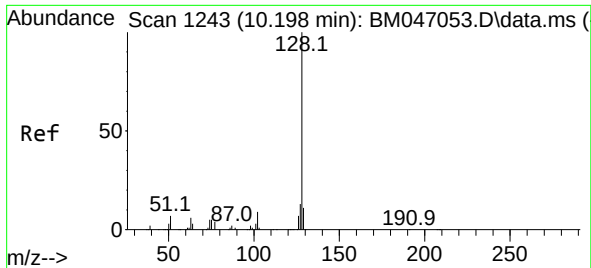

#30
Naphthalene
Concen: 4.049 ng/ul
RT: 10.198 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM047056.D
Acq: 07 Aug 2024 14:02

Instrument :
BNA_M
ClientSampleId :
C0AZ7

Tgt Ion:128 Resp: 253123
Ion Ratio Lower Upper
128 100
129 10.8 8.6 13.0
127 13.0 10.4 15.6

