

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080715\
 Data File : BM002292.D
 Acq On : 09 Aug 2015 00:56
 Operator : TP/UM
 Sample : G3126-04RE
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9D10RE

Quant Time: Aug 09 06:19:04 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080715MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Aug 09 06:16:29 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.92	152	370860	20.00	ng/ul	0.00
2) Naphthalene-d8	11.80	136	1809566	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.50	164	947257	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.21	188	1905323	20.00	ng/ul	0.00
17) Chrysene-d12	22.30	240	1501380	20.00	ng/ul	0.00
22) Perylene-d12	25.00	264	1195665	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	15.20	160	820006	8.36	ng/ul	0.00
10) Fluorene-d10	16.47	176	497592	7.29	ng/ul	0.00
14) Anthracene-d10	18.30	188	695655	7.52	ng/ul	0.00
18) Pyrene-d10	20.52	212	578948	7.95	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.81	264	374226	5.89	ng/ul	0.00
Target Compounds						
23) Benzo(b)fluoranthene	24.16	252	106784	1.44	ng/ul#	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080715\
Data File : BM002292.D
Acq On : 09 Aug 2015 00:56
Operator : TP/UM
Sample : G3126-04RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9D10RE

Quant Time: Aug 09 06:19:04 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080715MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Aug 09 06:16:29 2015
Response via : Initial Calibration

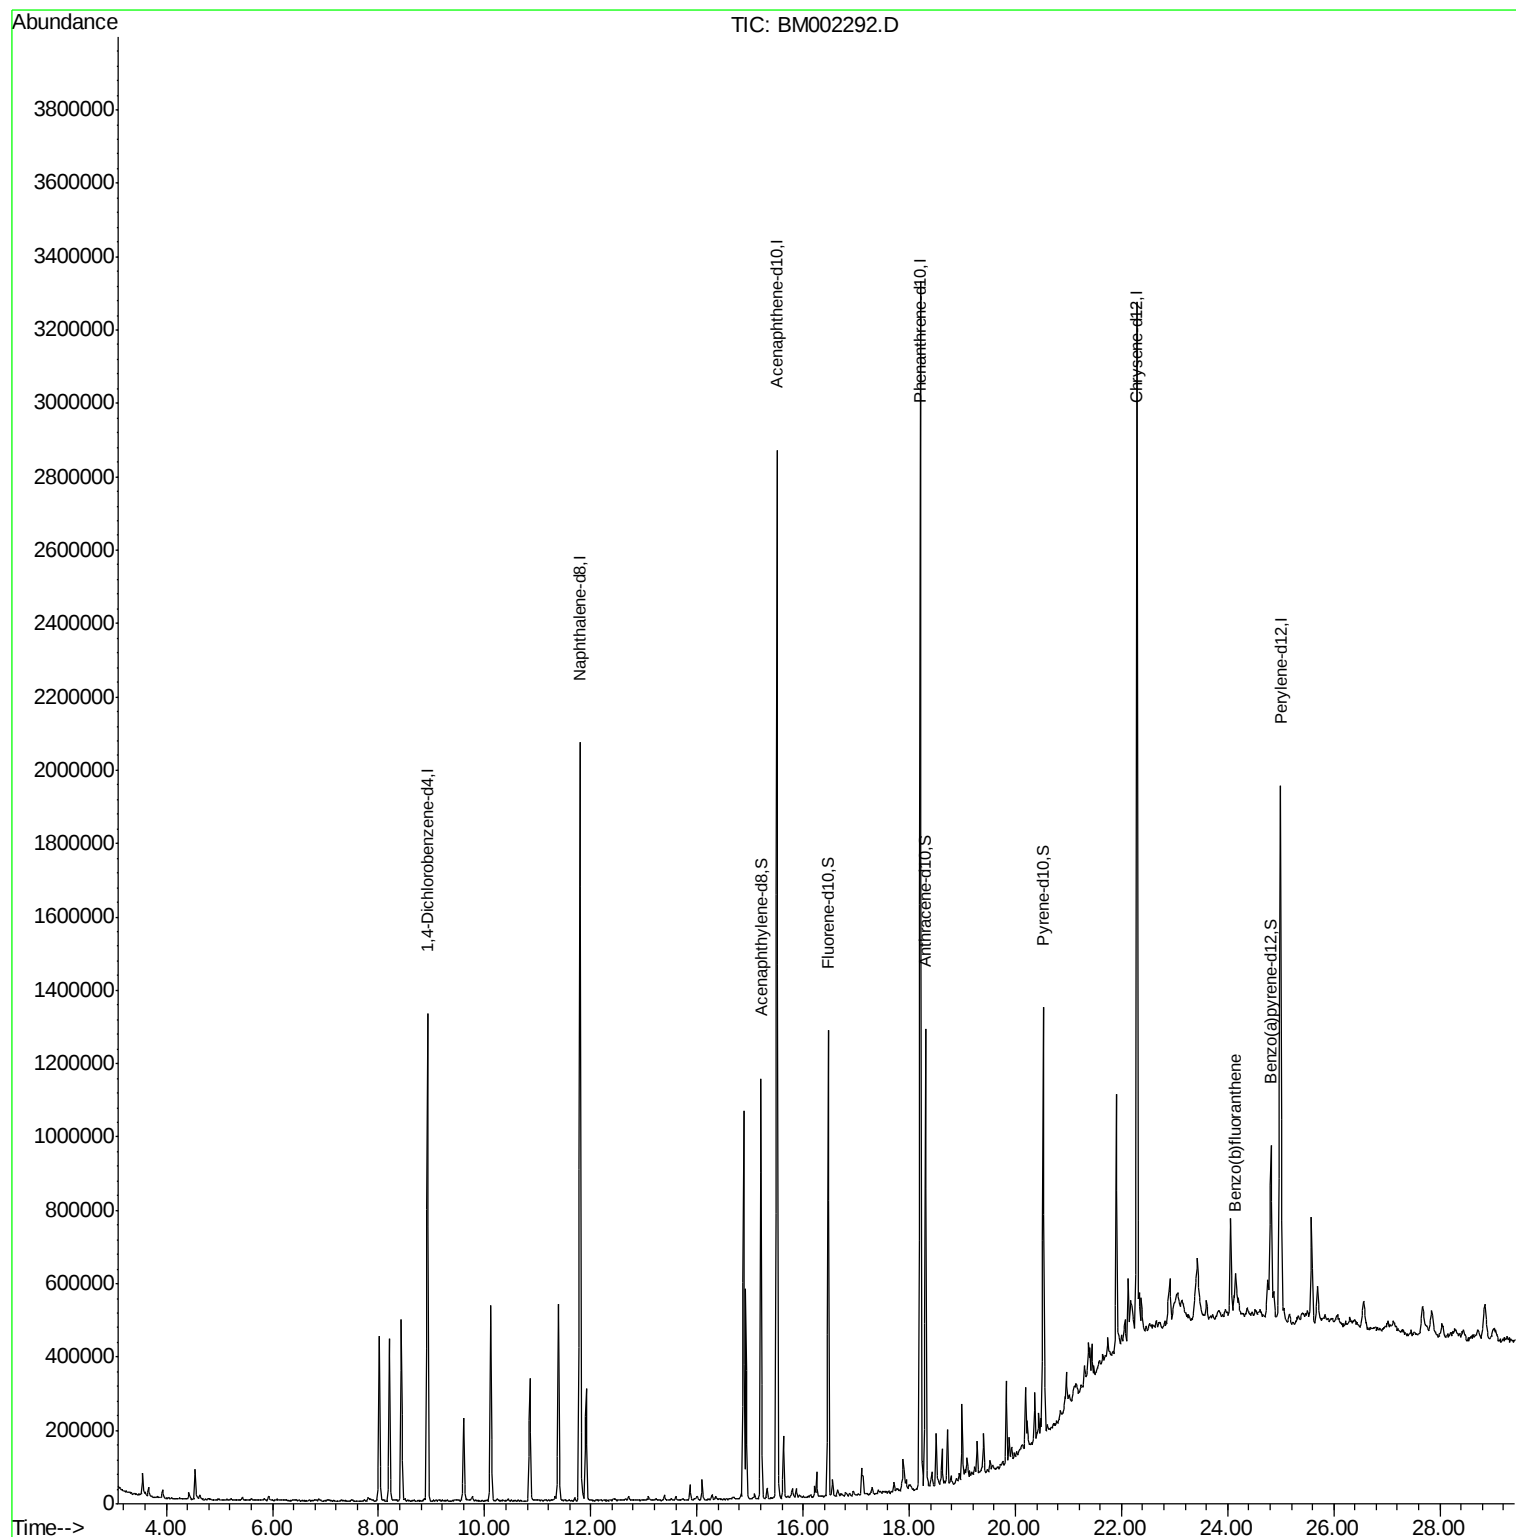

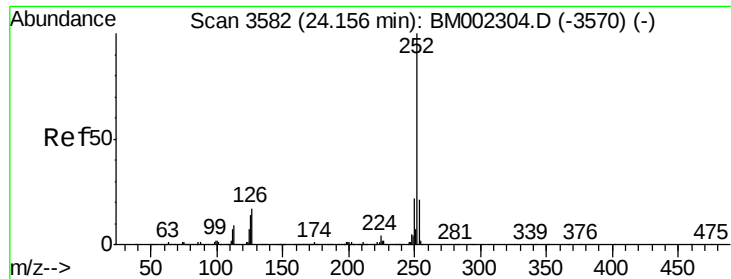

#23

Benzo(b)fluoranthene

Concen: 1.44 ng/ul

RT: 24.16 min Scan# 3582

Delta R.T. 0.00 min

Lab File: BM002292.D

Acq: 09 Aug 2015 00:56

Instrument :

BNA_M

ClientSampleId :

D9D10RE

Tgt Ion: 252 Resp: 106784

Ion Ratio Lower Upper

252 100

253 24.2 17.9 26.9

125 17.5 10.3 15.5#

