

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080717\
 Data File : BM011170.D
 Acq On : 08 Aug 2017 01:57
 Operator : SJ/JU
 Sample : I4560-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 N-STOCKPILE-COMP

Quant Time: Aug 08 02:34:28 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 17:29:06 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.31	152	100806	20.00	ng	-0.08
21) Naphthalene-d8	10.07	136	357107	20.00	ng	-0.08
38) Acenaphthene-d10	13.97	164	266237	20.00	ng	-0.08
63) Phenanthrene-d10	16.74	188	725982	20.00	ng	-0.07
75) Chrysene-d12	20.96	240	1084383	20.00	ng	-0.06
86) Perylene-d12	23.04	264	871325	20.00	ng	-0.09
System Monitoring Compounds						
5) 2-Fluorophenol	4.95	112	873240	146.44	ng	-0.08
7) Phenol-d6	6.52	99	1110437	131.06	ng	-0.08
23) Nitrobenzene-d5	8.46	82	1081688	113.68	ng	-0.08
41) 2,4,6-Tribromophenol	15.49	330	649225	152.14	ng	-0.07
44) 2-Fluorobiphenyl	12.59	172	1914810	90.20	ng	-0.08
78) Terphenyl-d14	19.41	244	4790395	87.51	ng	-0.06


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080717\
Data File : BM011170.D
Acq On : 08 Aug 2017 01:57
Operator : SJ/JU
Sample : I4560-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
N-STOCKPILE-COMP

Quant Time: Aug 08 02:34:28 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

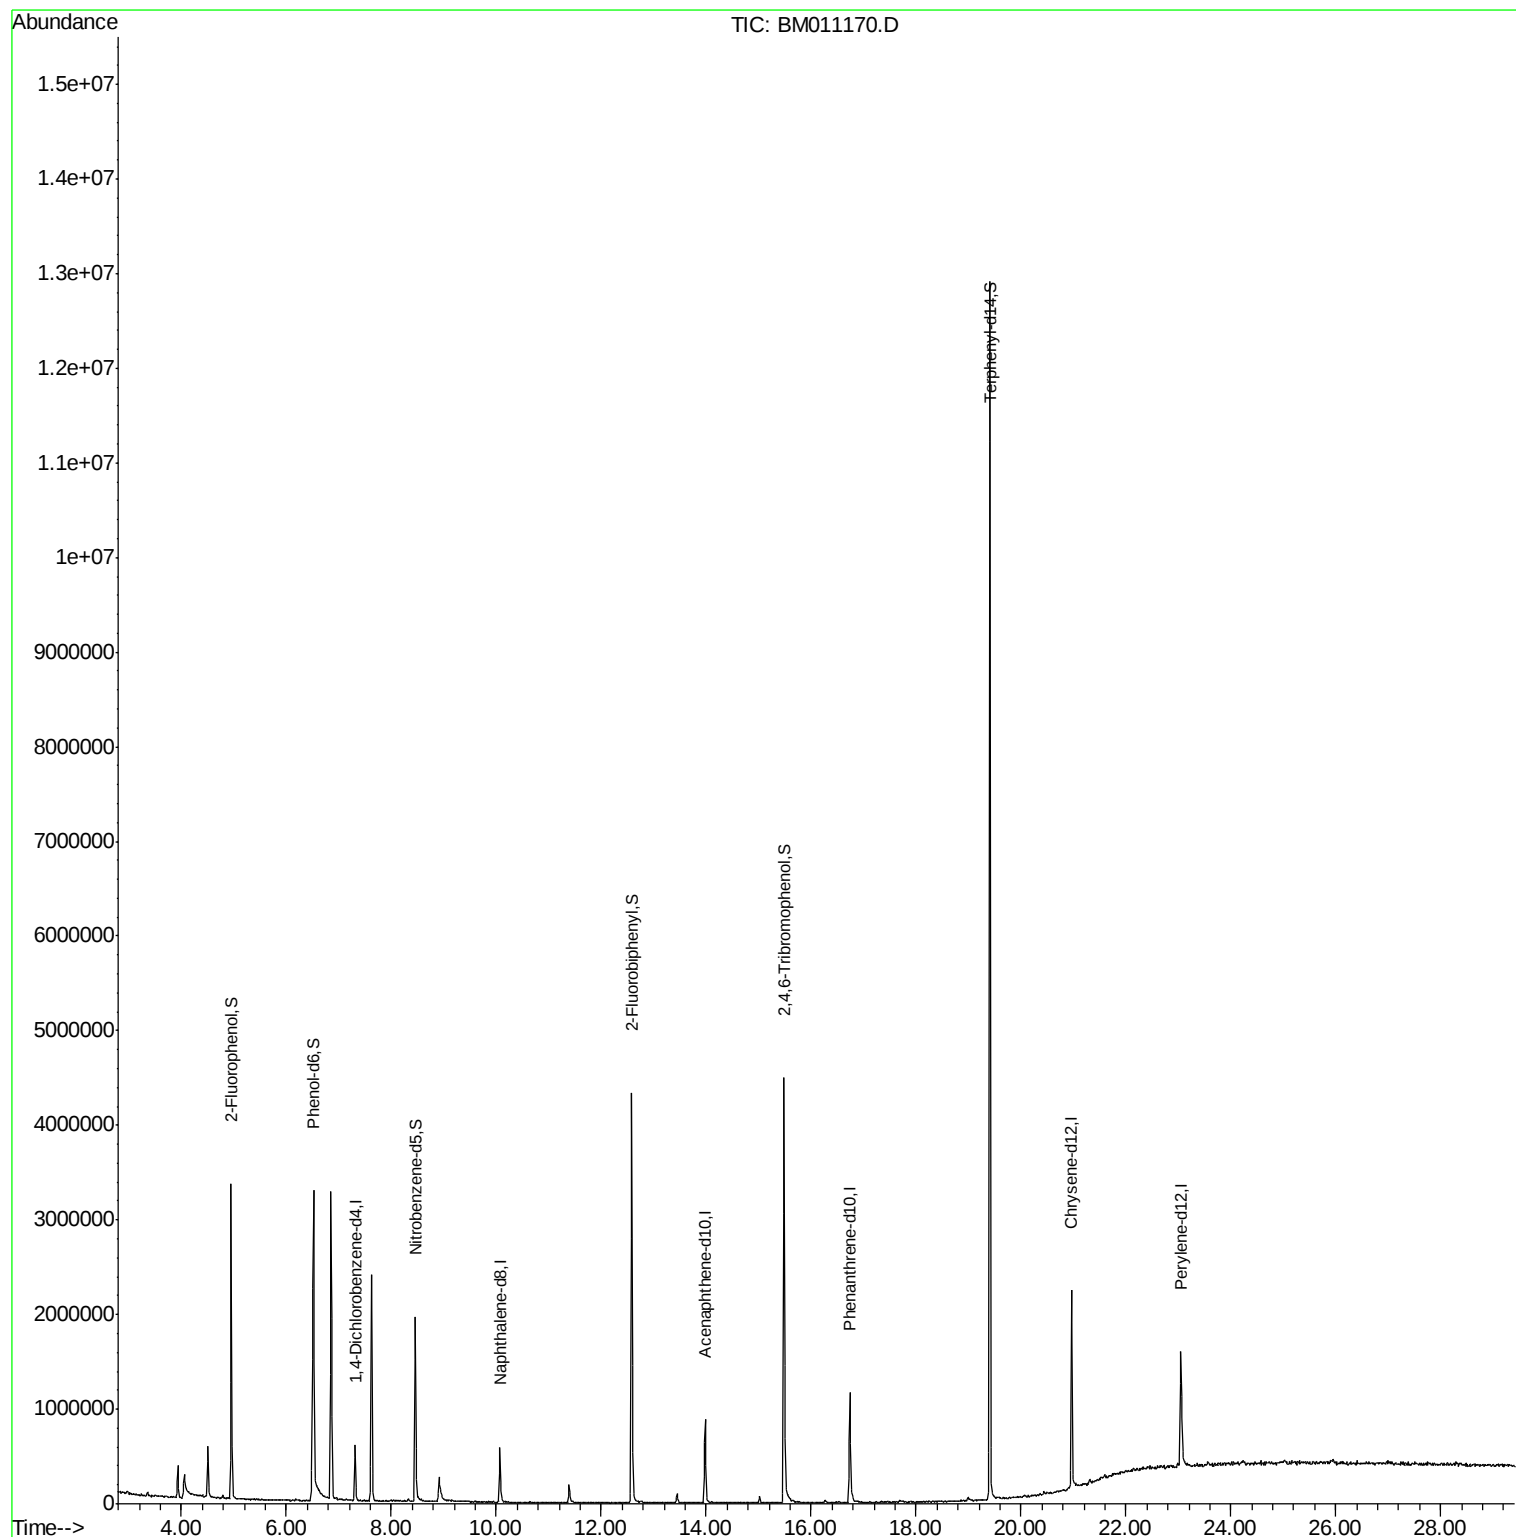




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.31 min Scan# 769
Delta R.T. -0.08 min
Lab File: BM011170.D
Acq: 08 Aug 2017 01:57

Instrument :
BNA_M
ClientSampleId :
N-STOCKPILE-COMP

Tot Ion:152 Resp: 100806
Ion Ratio Lower Upper
152 100
150 152.8 119.5 179.3
115 64.4 43.0 64.4#

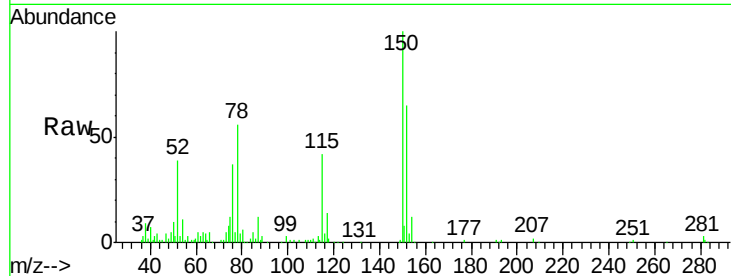


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

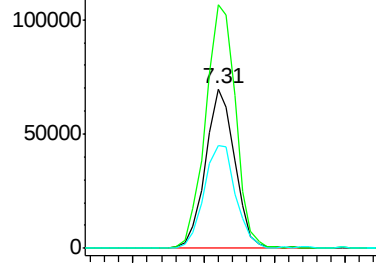



#5


2-Fluorophenol
Concen: 146.44 ng
RT: 4.95 min Scan# 368
Delta R.T. -0.08 min
Lab File: BM011170.D
Acq: 08 Aug 2017 01:57

Tgt Ion:112 Resp: 873240
Ion Ratio Lower Upper
112 100
64 79.2 38.6 57.8#
63 52.5 19.3 28.9#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

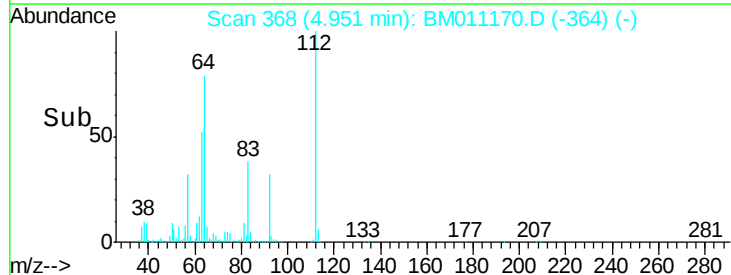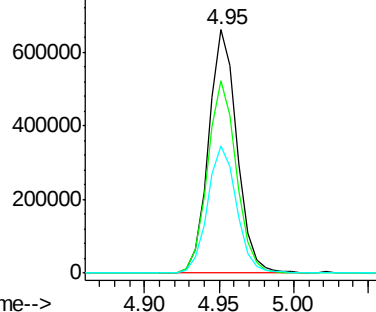



#7

Phenol-d6

Concen: 131.06 ng

RT: 6.52 min Scan# 634

Delta R.T. -0.08 min

Lab File: BM011170.D

Acq: 08 Aug 2017 01:57

Instrument :

BNA_M

ClientSampleId :

N-STOCKPILE-COMP


Tot Ion: 99 Resp: 1110437

Ion Ratio Lower Upper

99 100

42 27.0 11.0 16.4#

71 67.5 23.4 35.2#






Abundance Ion 99.00 (98.70 to 99.70): BM011170.D (-630) (-)

Ion 42.00 (41.70 to 42.70): BM011170.D (-630) (-)

Ion 71.00 (70.70 to 71.70): BM011170.D (-630) (-)

Time-->

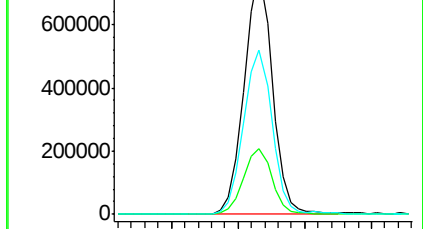

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.07 min Scan# 1238

Delta R.T. -0.08 min

Lab File: BM011170.D

Acq: 08 Aug 2017 01:57

Tgt Ion: 136 Resp: 357107


Ion Ratio Lower Upper

136 100

137 10.8 8.7 13.1

54 10.6 4.6 6.8#

68 7.2 3.7 5.5#





Abundance Ion 136.00 (135.70 to 136.70): BM011170.D (-1235) (-)


Ion 137.00 (136.70 to 137.70): BM011170.D (-1235) (-)

Ion 54.00 (53.70 to 54.70): BM011170.D (-1235) (-)

Ion 68.00 (67.70 to 68.70): BM011170.D (-1235) (-)

Time-->

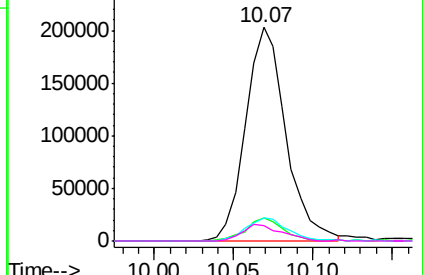







#23
 Nitrobenzene-d5
 Concen: 113.68 ng
 RT: 8.46 min Scan# 964
 Delta R.T. -0.08 min
 Lab File: BM011170.D
 Acq: 08 Aug 2017 01:57

Instrument :
 BNA_M
 ClientSampleId :
 N-STOCKPILE-COMP

Tot Ion: 82 Resp: 1081688




Ion	Ratio	Lower	Upper
82	100		
128	23.7	32.8	49.2#
54	52.5	40.6	60.8

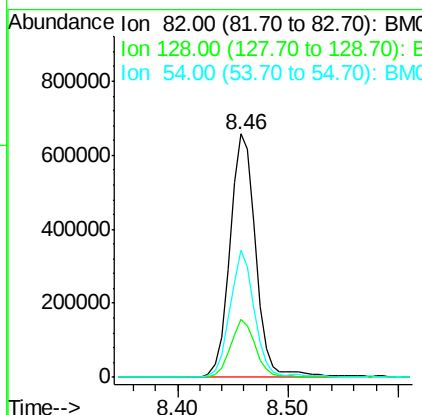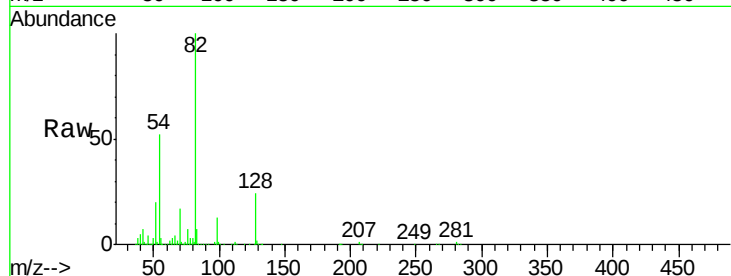


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 13.97 min Scan# 1902
 Delta R.T. -0.08 min
 Lab File: BM011170.D
 Acq: 08 Aug 2017 01:57

Tgt Ion: 164 Resp: 266237

Ion	Ratio	Lower	Upper
164	100		
162	102.1	82.4	123.6
160	44.5	35.8	53.6

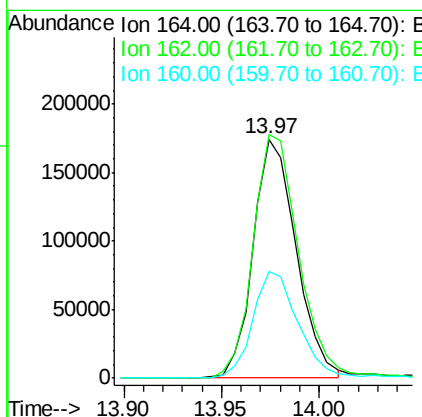







#41
 2,4,6-Tribromophenol
 Concen: 152.14 ng
 RT: 15.49 min Scan# 2159
 Delta R.T. -0.07 min
 Lab File: BM011170.D
 Acq: 08 Aug 2017 01:57

Instrument :
 BNA_M
 ClientSampleId :
 N-STOCKPILE-COMP

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.3	0.0	0.0#
141	48.9	0.0	0.0#

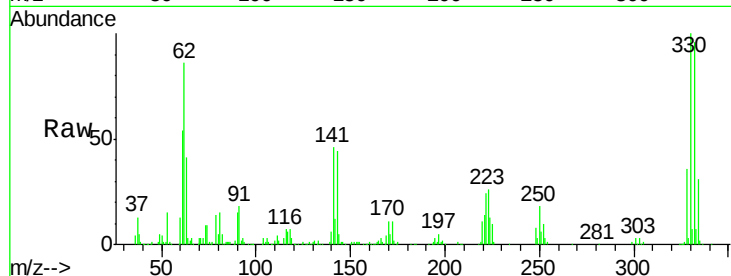


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

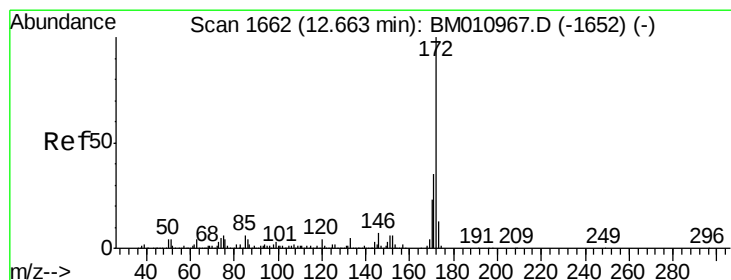
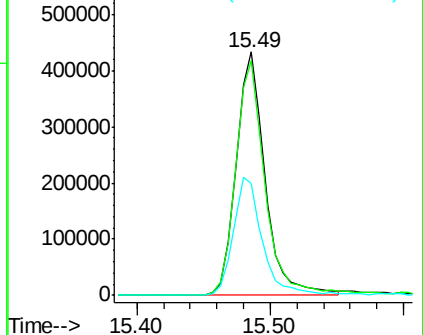



#44
 2-Fluorobiphenyl
 Concen: 90.20 ng
 RT: 12.59 min Scan# 1666
 Delta R.T. -0.08 min
 Lab File: BM011170.D
 Acq: 08 Aug 2017 01:57

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	28.5	42.7
170	23.0	18.8	28.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




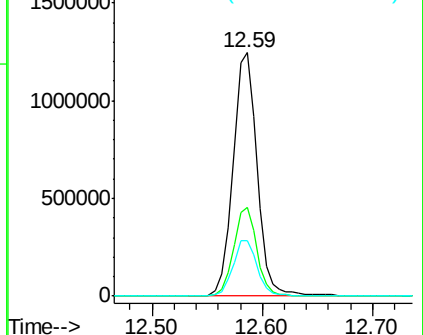




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 16.74 min Scan# 2372
Delta R.T. -0.07 min
Lab File: BM011170.D
Acq: 08 Aug 2017 01:57




Instrument :
BNA_M
ClientSampleId :
N-STOCKPILE-COMP


Tot Ion:188 Resp: 725982
Ion Ratio Lower Upper
188 100
94 7.5 8.7 13.1#
80 9.2 9.3 13.9#

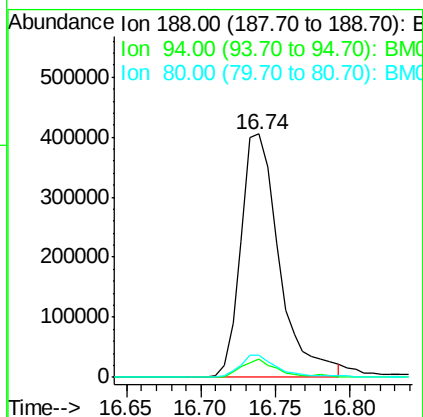

#75
Chrysene-d12
Concen: 20.00 ng
RT: 20.96 min Scan# 3090
Delta R.T. -0.06 min
Lab File: BM011170.D
Acq: 08 Aug 2017 01:57

Tgt Ion:240 Resp: 1084383
Ion Ratio Lower Upper
240 100
120 4.6 8.2 12.2#
236 24.6 20.0 30.0

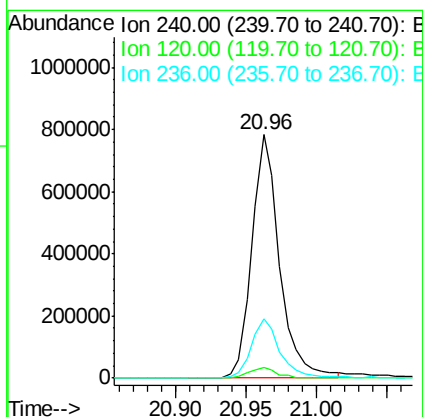


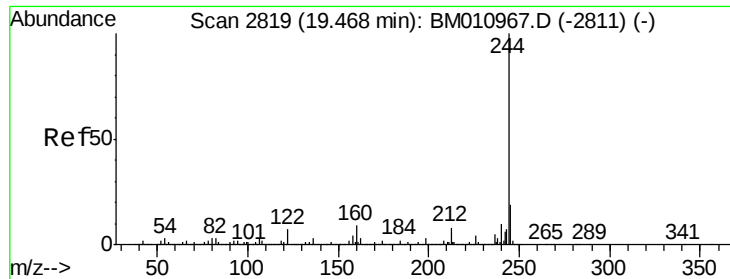




#78
 Terphenyl-d14
 Concen: 87.51 ng
 RT: 19.41 min Scan# 2826
 Delta R.T. -0.06 min
 Lab File: BM011170.D
 Acq: 08 Aug 2017 01:57

Instrument :
 BNA_M
 ClientSampleId :
 N-STOCKPILE-COMP

Tot Ion:244 Resp: 4790395
 Ion Ratio Lower Upper
 244 100
 212 9.0 4.9 7.3#
 122 6.6 6.2 9.4

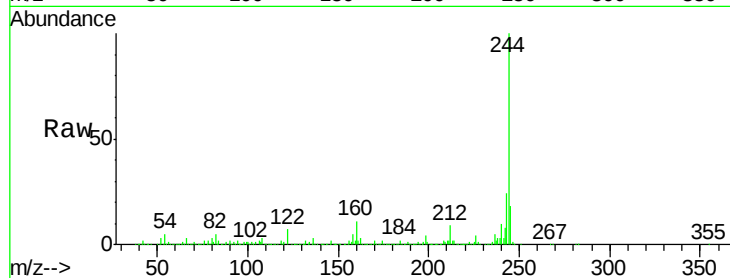


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

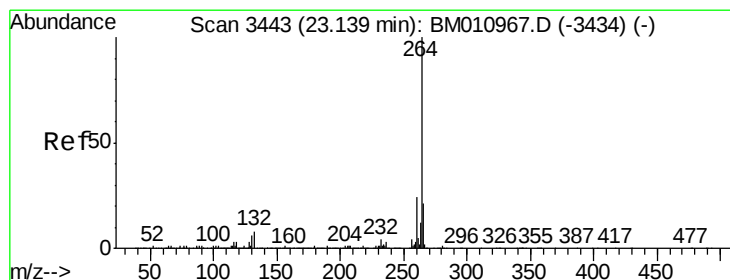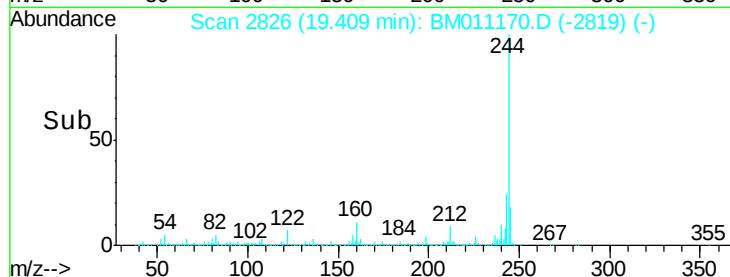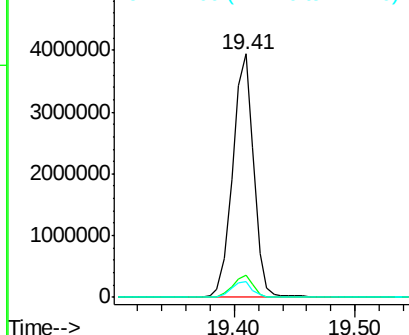

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 23.04 min Scan# 3444
 Delta R.T. -0.09 min
 Lab File: BM011170.D
 Acq: 08 Aug 2017 01:57

Tgt Ion:264 Resp: 871325
 Ion Ratio Lower Upper
 264 100
 260 24.0 18.6 27.8
 265 20.5 17.3 25.9

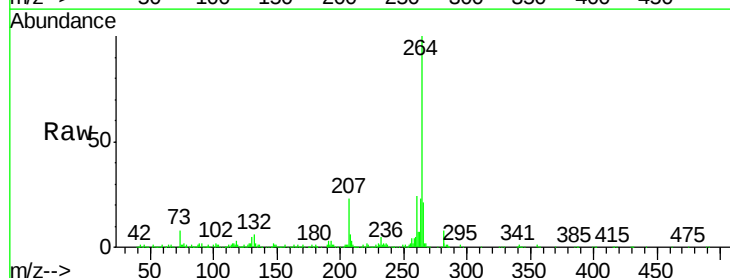

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

