
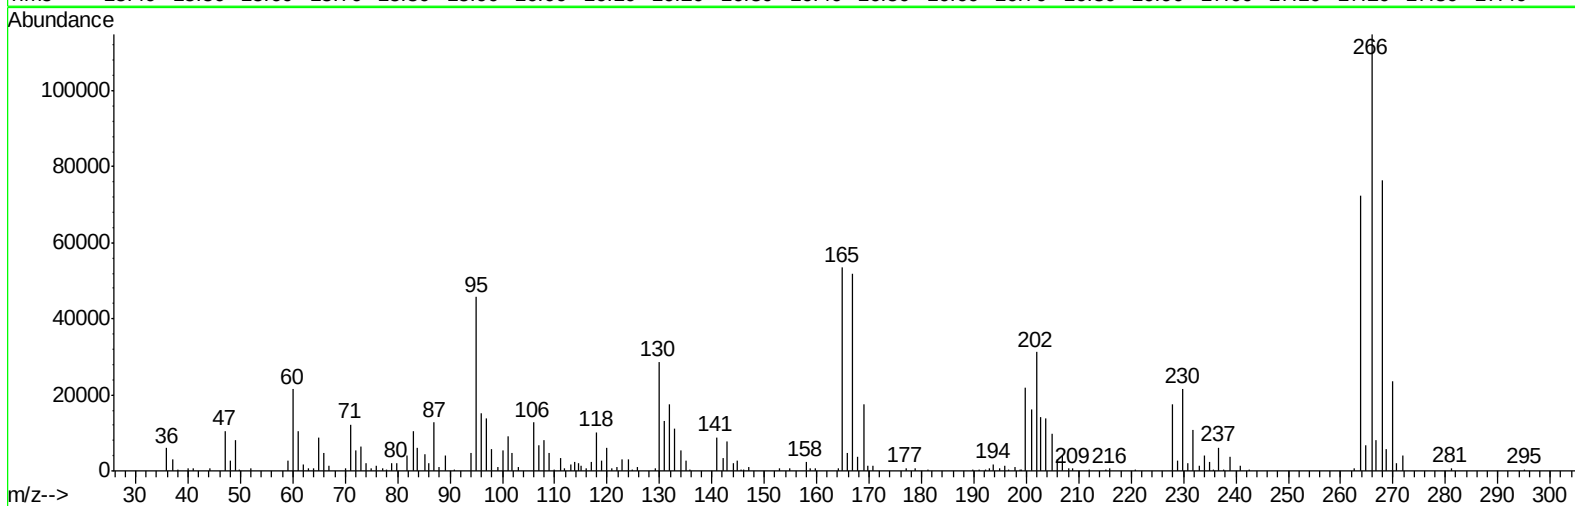


Data Path : Z:\HPCHEM1\BNA M\DATA\BM080717\
Data File : BM011152.D
Acq On : 07 Aug 2017 15:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 03:55:21 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

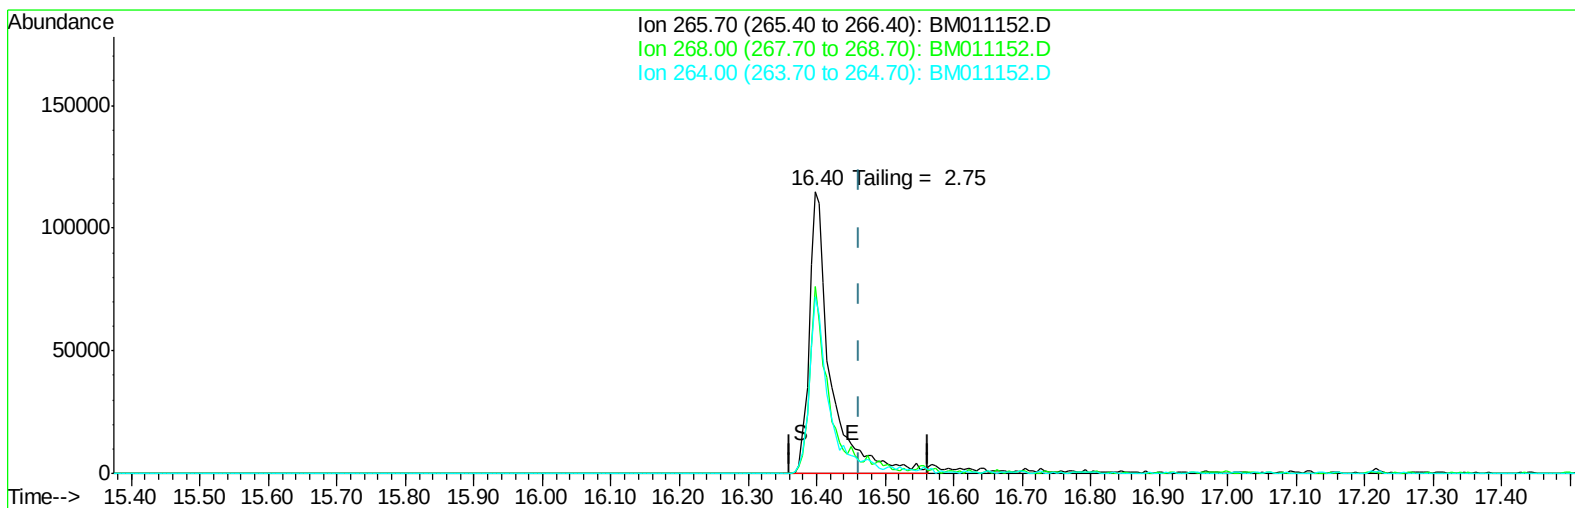

TIC: BM011152.D

(69) Pentachlorophenol (C)



16.398min (-0.065) 0.00ng

response 213234

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	66.47
264.00	61.20	62.95
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA M\DATA\BM080717\
Data File : BM011152.D
Acq On    : 07 Aug 2017  15:04
Operator  : SJ/JU
Sample    : DFTPP
Misc      :
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Aug 08 03:55:21 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

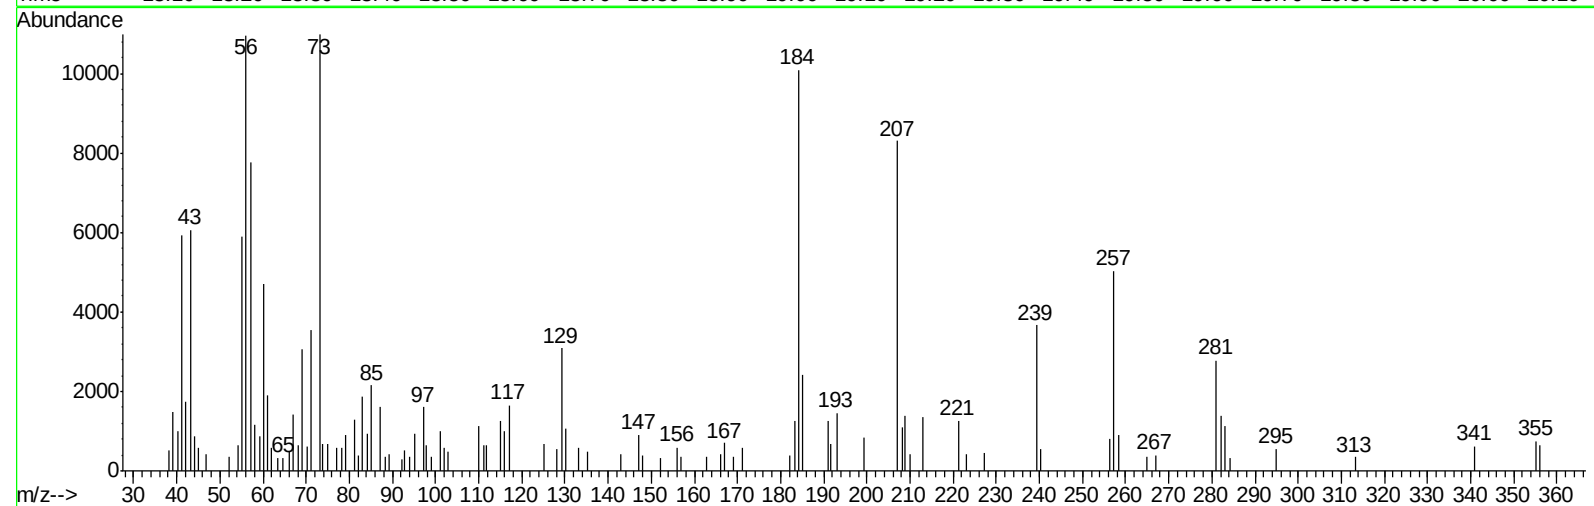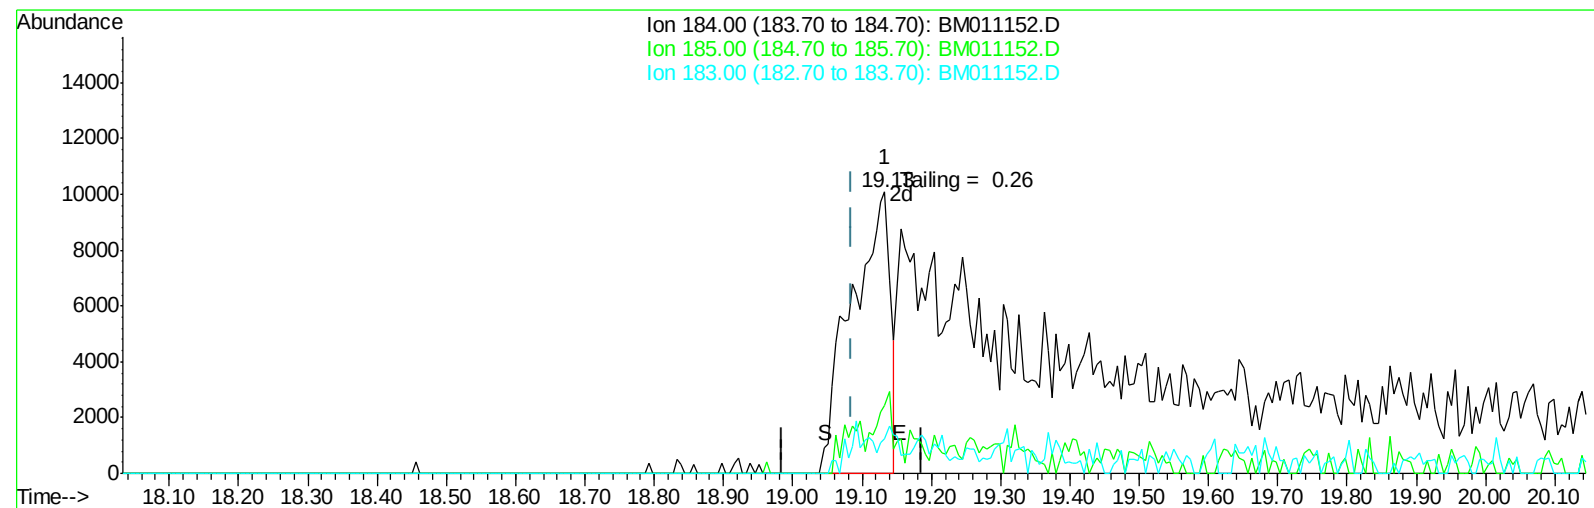

TIC: BM011152.D

(76) Benzidine

19.133min (+0.047) 5376.22ng

response 38327

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	23.95#
183.00	11.10	12.33
0.00	0.00	0.00