

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080717\
 Data File : BM011162.D
 Acq On : 07 Aug 2017 21:07
 Operator : SJ/JU
 Sample : I4610-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PL-02-080317-C

Quant Time: Aug 08 02:17:59 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 26 17:29:06 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.32	152	128287	20.00	ng	-0.08
21) Naphthalene-d8	10.07	136	430004	20.00	ng	-0.08
38) Acenaphthene-d10	13.98	164	323419	20.00	ng	-0.07
63) Phenanthrene-d10	16.74	188	858185	20.00	ng	-0.07
75) Chrysene-d12	20.96	240	1123317	20.00	ng	-0.06
86) Perylene-d12	23.05	264	1218972	20.00	ng	-0.09
System Monitoring Compounds						
5) 2-Fluorophenol	4.96	112	1229481	162.01	ng	-0.07
7) Phenol-d6	6.52	99	1561099	144.78	ng	-0.07
23) Nitrobenzene-d5	8.46	82	1525785	133.17	ng	-0.08
41) 2,4,6-Tribromophenol	15.49	330	908328	175.23	ng	-0.07
44) 2-Fluorobiphenyl	12.59	172	2729490	105.84	ng	-0.08
78) Terphenyl-d14	19.41	244	6200720	109.34	ng	-0.06


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080717\
Data File : BM011162.D
Acq On : 07 Aug 2017 21:07
Operator : SJ/JU
Sample : I4610-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PL-02-080317-C

Quant Time: Aug 08 02:17:59 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

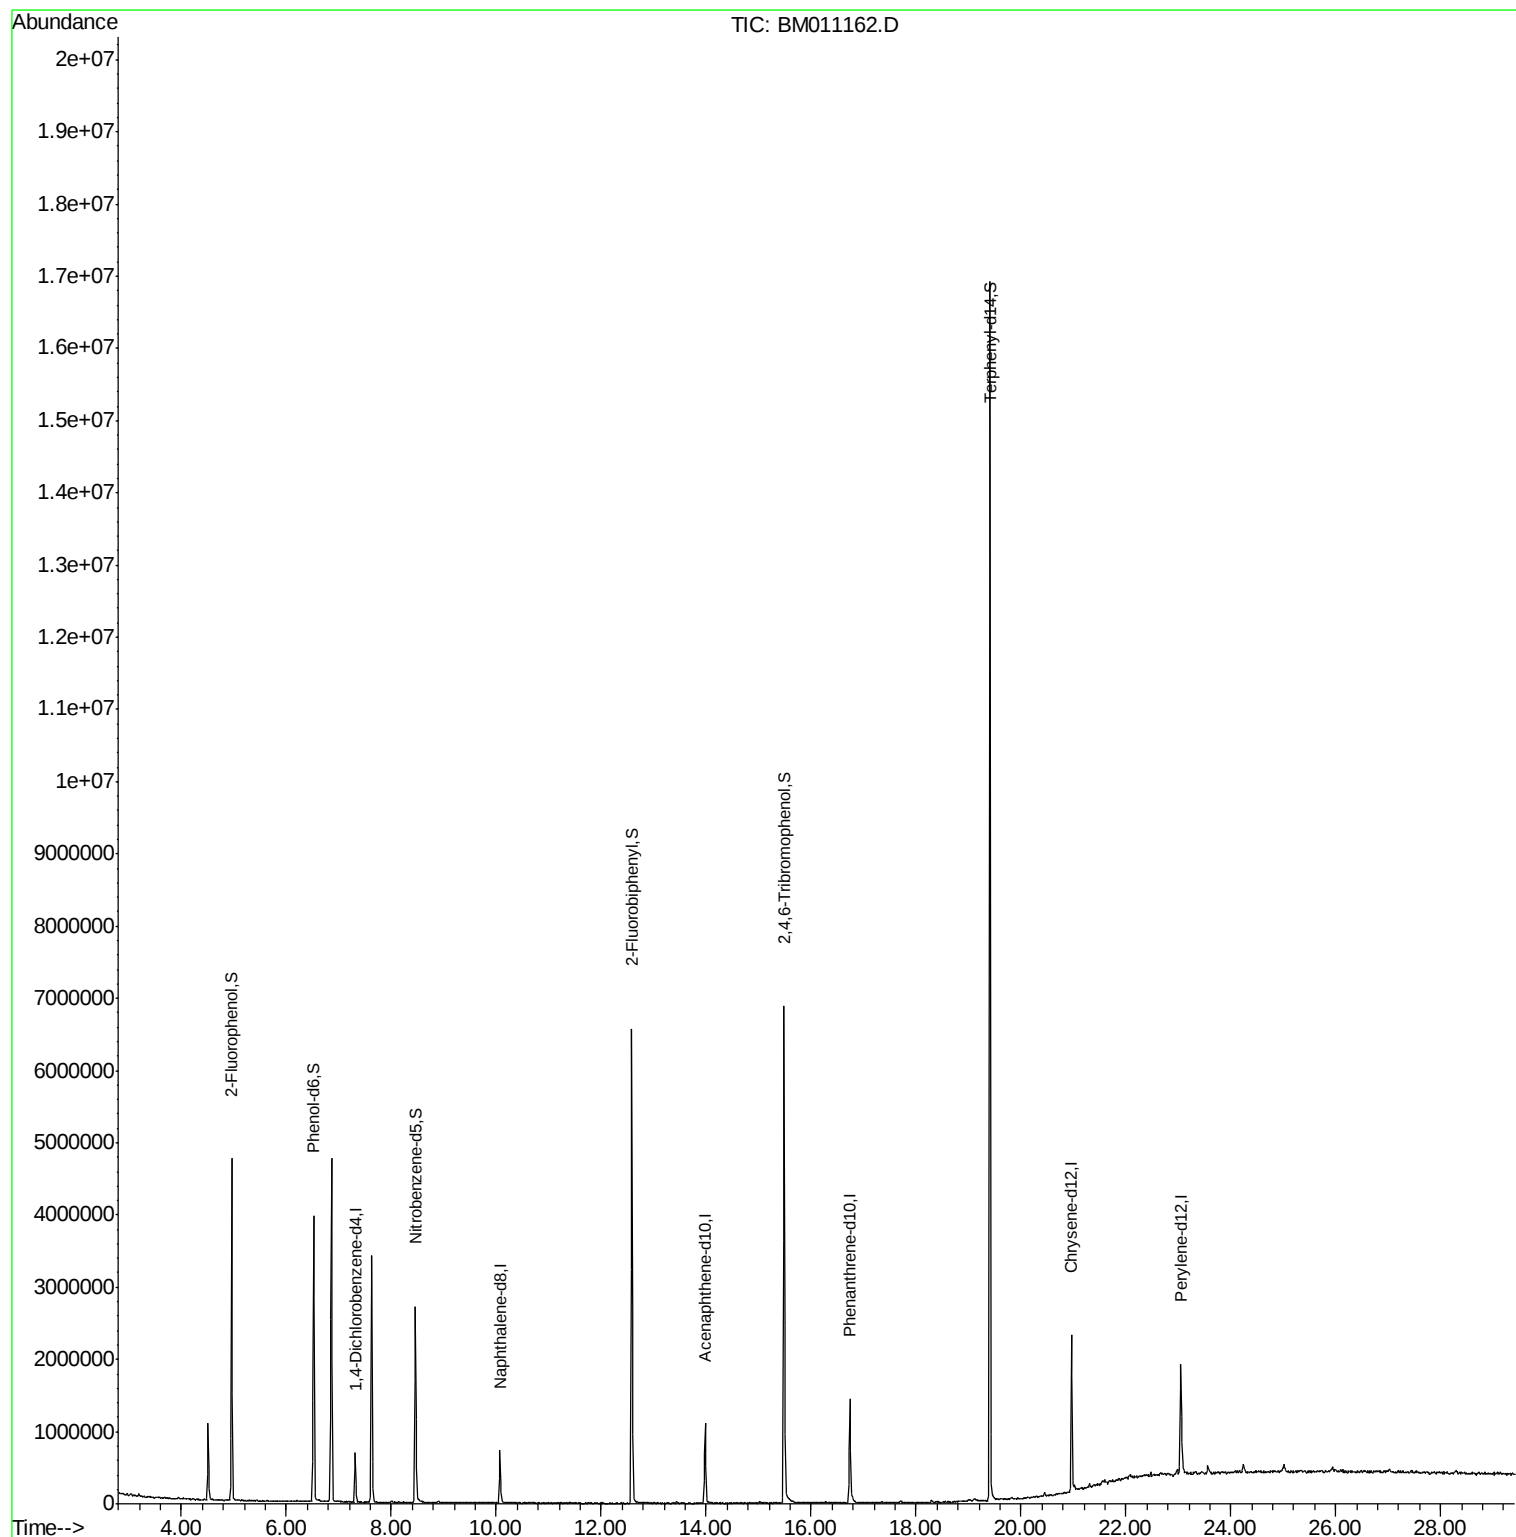

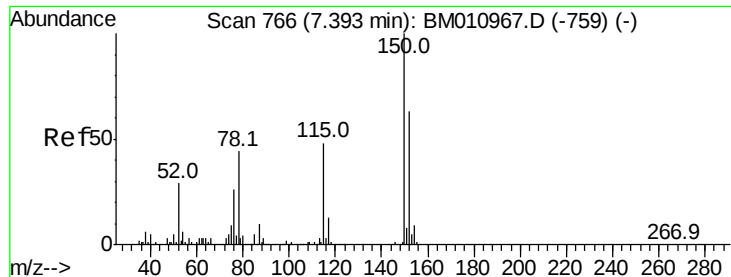


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.32 min Scan# 770
Delta R.T. -0.08 min
Lab File: BM011162.D
Acq: 07 Aug 2017 21:07

Instrument :
BNA_M
ClientSampleId :
PL-02-080317-C

Tot Ion:152 Resp: 128287
Ion Ratio Lower Upper
152 100
150 143.2 119.5 179.3
115 71.2 43.0 64.4#

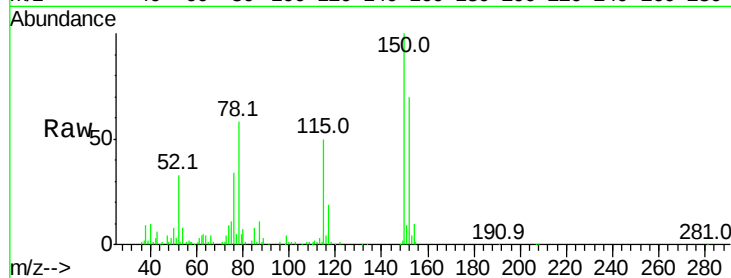


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

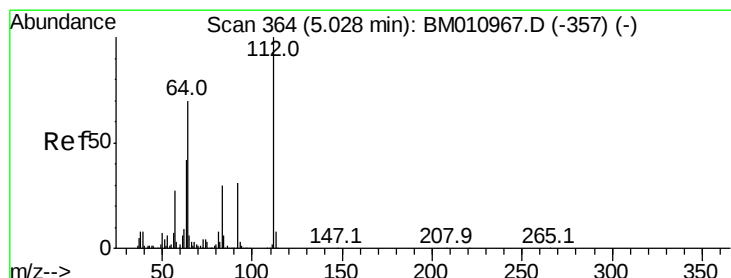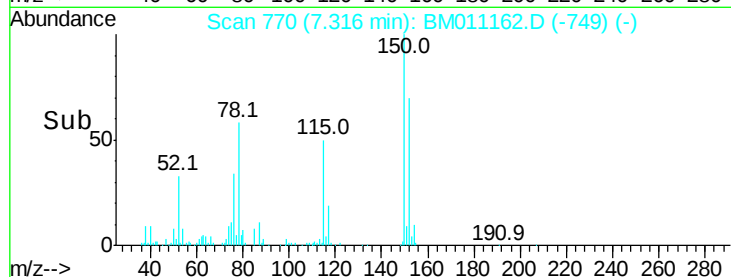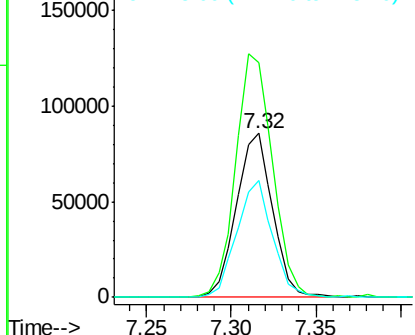



#5

2-Fluorophenol
Concen: 162.009 ng
RT: 4.96 min Scan# 369
Delta R.T. -0.07 min
Lab File: BM011162.D
Acq: 07 Aug 2017 21:07

Tgt Ion:112 Resp: 1229481
Ion Ratio Lower Upper
112 100
64 78.8 38.6 57.8#
63 53.2 19.3 28.9#

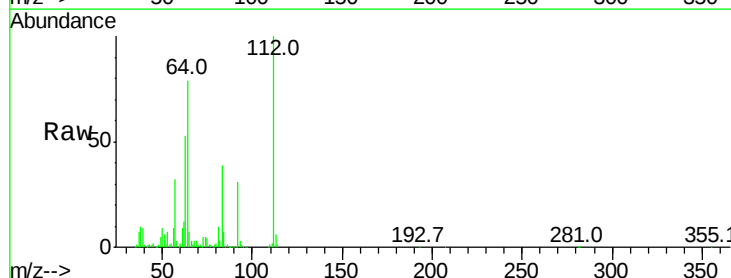

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

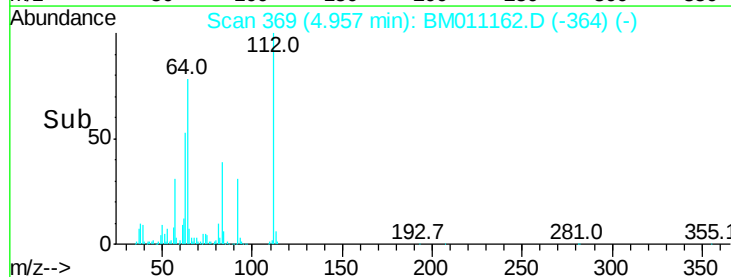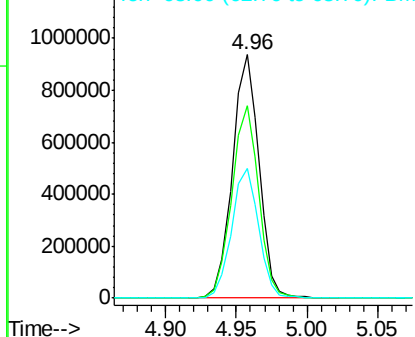



#7

Phenol-d6

Concen: 144.780 ng

RT: 6.52 min Scan# 635

Delta R.T. -0.07 min

Lab File: BM011162.D

Acq: 07 Aug 2017 21:07

Instrument :

BNA_M

ClientSampleId :

PL-02-080317-C





Tot Ion: 99 Resp: 1561099

Ion Ratio Lower Upper

99 100

42 26.8 11.0 16.4#

71 67.1 23.4 35.2#

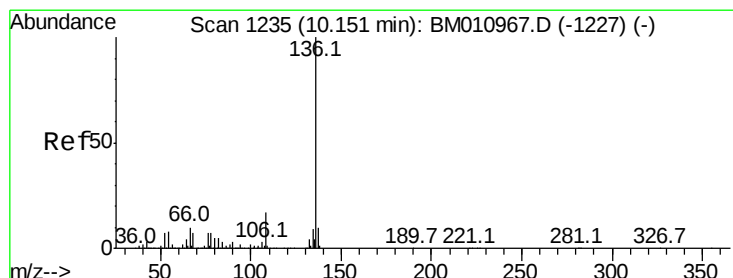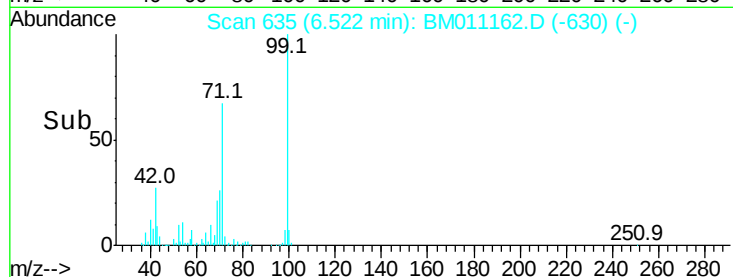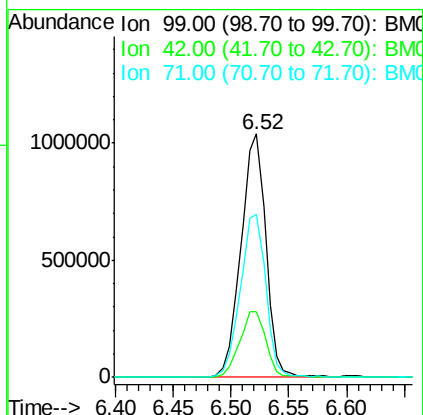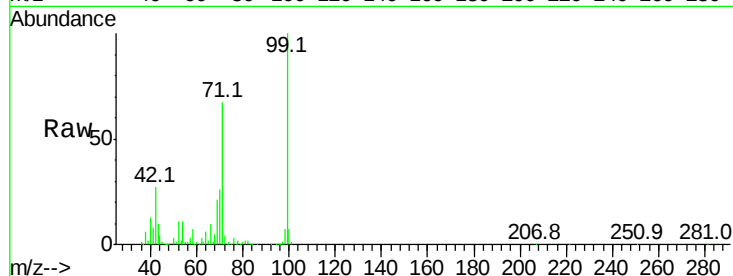

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.07 min Scan# 1238

Delta R.T. -0.08 min

Lab File: BM011162.D

Acq: 07 Aug 2017 21:07

Tgt Ion: 136 Resp: 430004




Ion Ratio Lower Upper

136 100

137 11.6 8.7 13.1

54 11.8 4.6 6.8#

68 7.8 3.7 5.5#

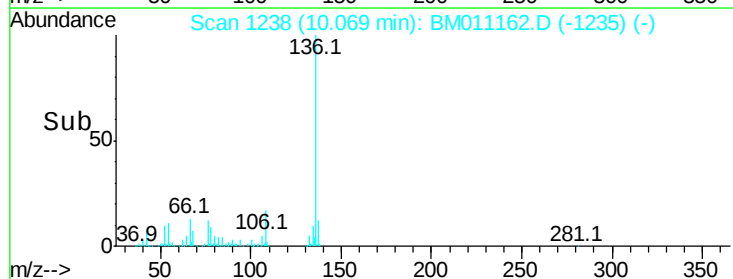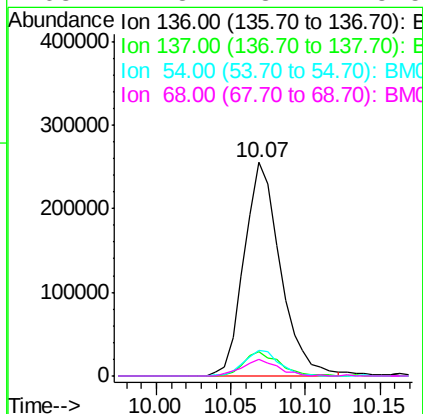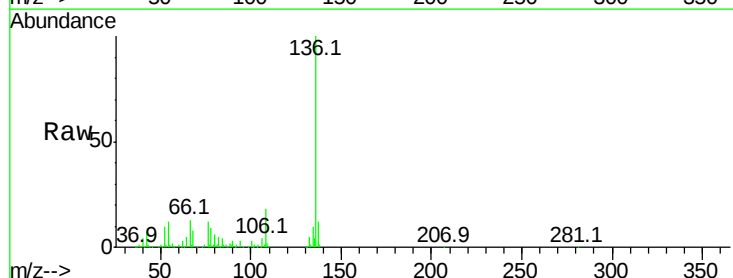







#23
 Nitrobenzene-d5
 Concen: 133.174 ng
 RT: 8.46 min Scan# 965
 Delta R.T. -0.08 min
 Lab File: BM011162.D
 Acq: 07 Aug 2017 21:07

Instrument :
 BNA_M
 ClientSampleId :
 PL-02-080317-C

Tot Ion: 82 Resp: 1525785




Ion	Ratio	Lower	Upper
82	100		
128	22.6	32.8	49.2#
54	50.9	40.6	60.8

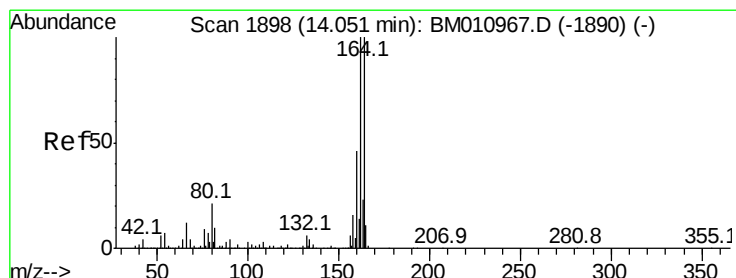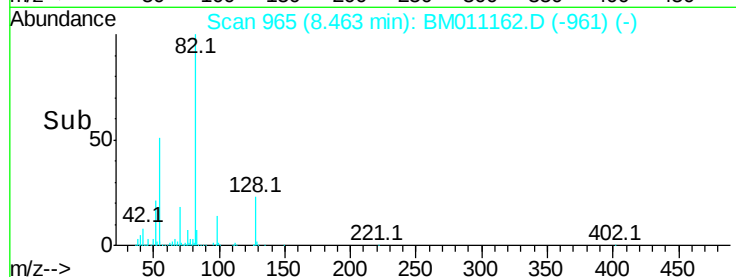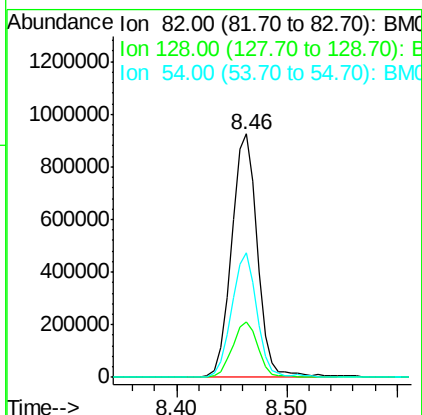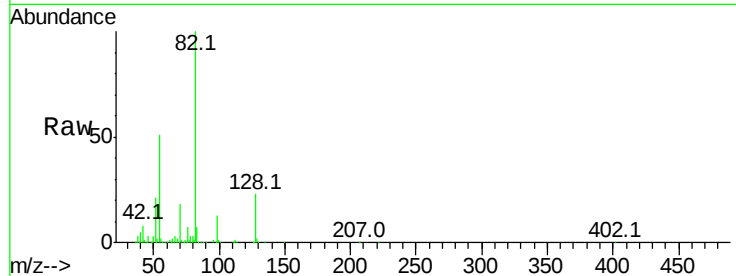


#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 13.98 min Scan# 1903
 Delta R.T. -0.07 min
 Lab File: BM011162.D
 Acq: 07 Aug 2017 21:07

Tgt Ion: 164 Resp: 323419

Ion	Ratio	Lower	Upper
164	100		
162	102.8	82.4	123.6
160	45.8	35.8	53.6

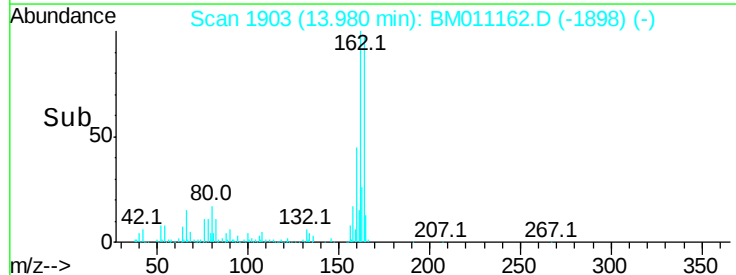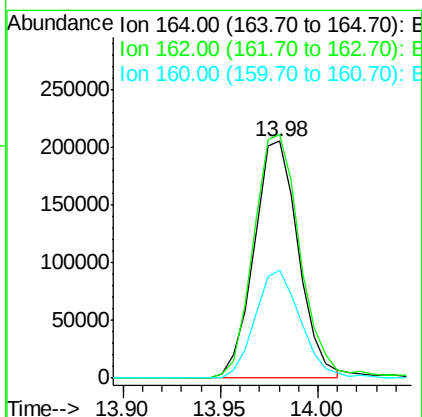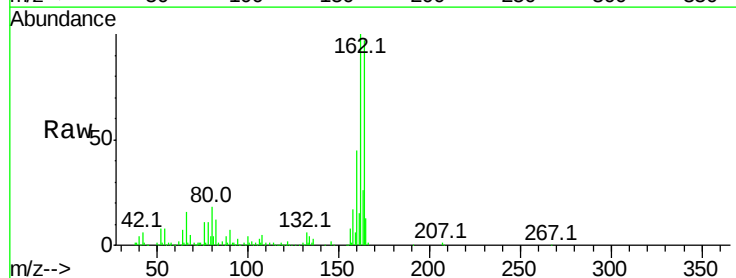


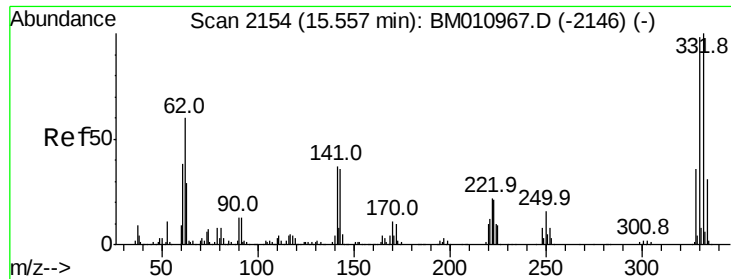



#41
 2,4,6-Tribromophenol
 Concen: 175.227 ng
 RT: 15.49 min Scan# 2159
 Delta R.T. -0.07 min
 Lab File: BM011162.D
 Acq: 07 Aug 2017 21:07

Instrument :
 BNA_M
 ClientSampleId :
 PL-02-080317-C

Tot Ion	Ratio	Lower	Upper
330	100		
332	99.4	0.0	0.0#
141	48.7	0.0	0.0#

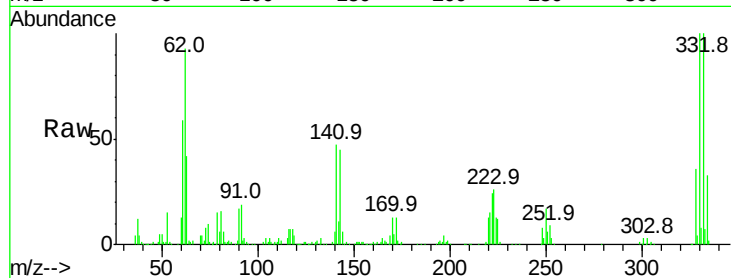


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

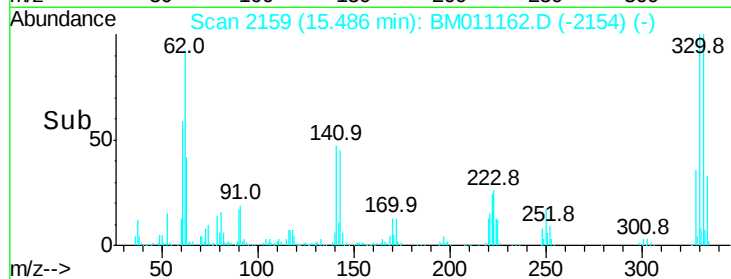
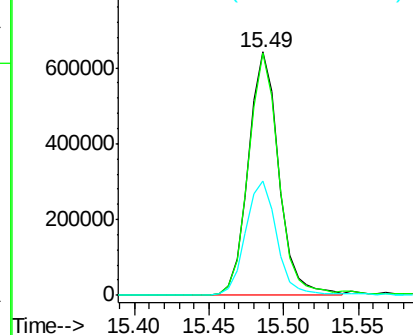



#44
 2-Fluorobiphenyl
 Concen: 105.843 ng
 RT: 12.59 min Scan# 1666
 Delta R.T. -0.08 min
 Lab File: BM011162.D
 Acq: 07 Aug 2017 21:07

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	28.5	42.7
170	23.5	18.8	28.2

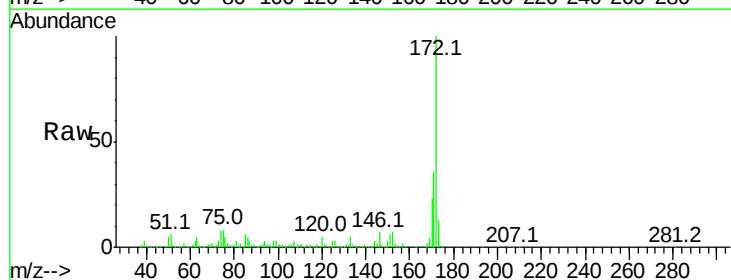

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



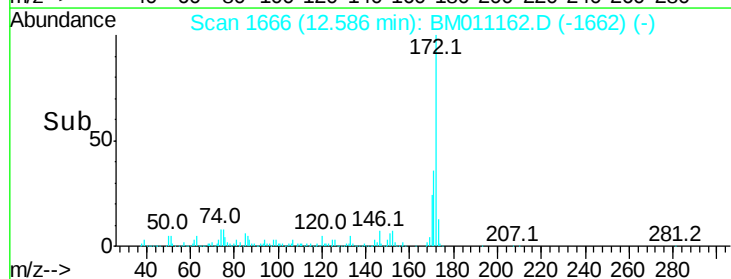
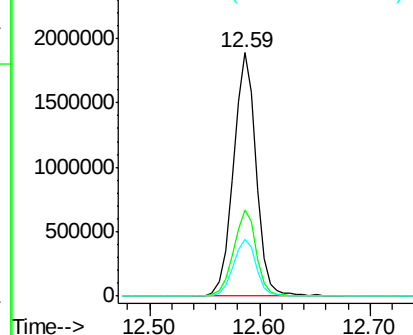


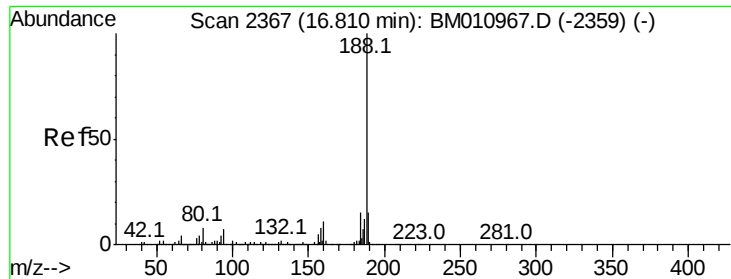

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.74 min Scan# 2372
Delta R.T. -0.07 min
Lab File: BM011162.D
Acq: 07 Aug 2017 21:07




Instrument :
BNA_M
ClientSampleId :
PL-02-080317-C


Tot Ion:188 Resp: 858185
Ion Ratio Lower Upper
188 100
94 6.2 8.7 13.1#
80 8.5 9.3 13.9#

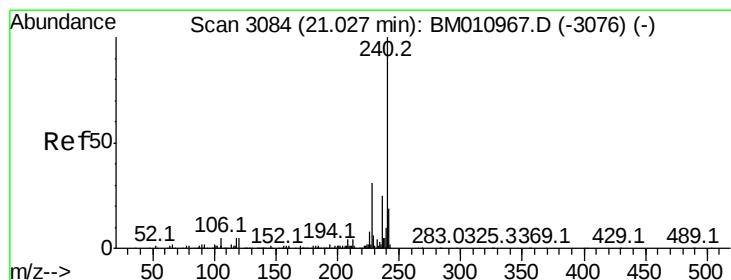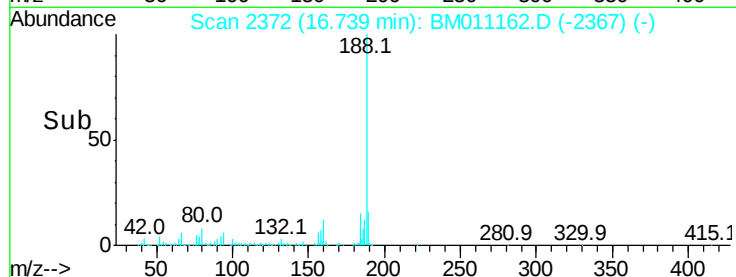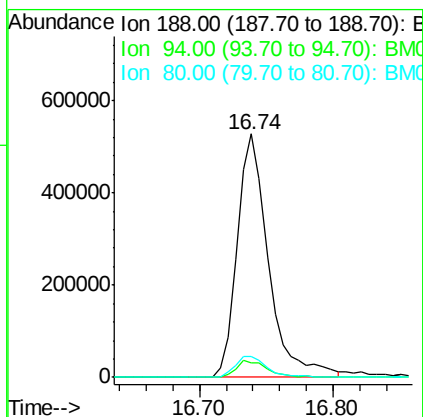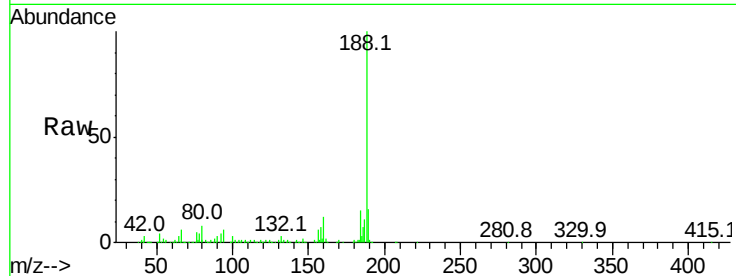

#75
Chrysene-d12
Concen: 20.000 ng
RT: 20.96 min Scan# 3090
Delta R.T. -0.06 min
Lab File: BM011162.D
Acq: 07 Aug 2017 21:07

Tgt Ion:240 Resp: 1123317
Ion Ratio Lower Upper
240 100
120 4.4 8.2 12.2#
236 26.0 20.0 30.0

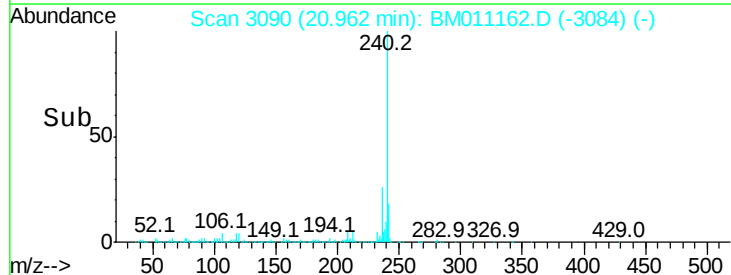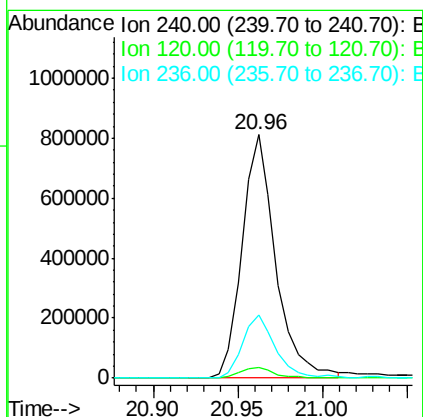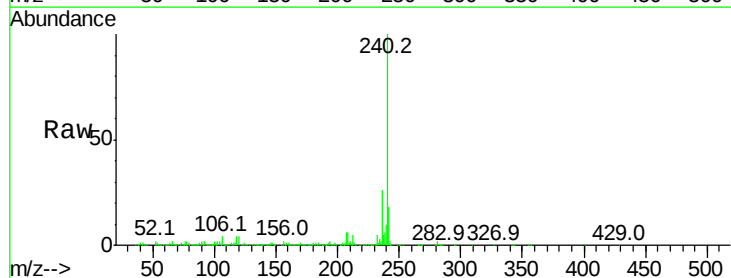

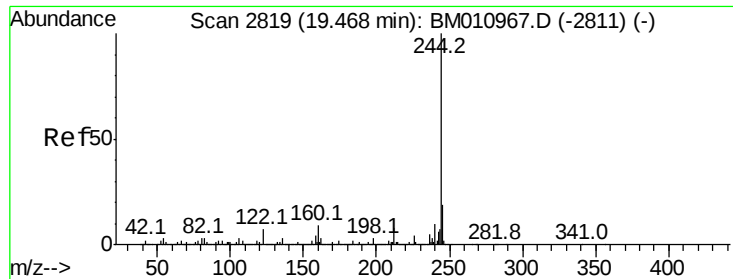

#78

Terphenyl-d14

Concen: 109.344 ng

RT: 19.41 min Scan# 2826

Delta R.T. -0.06 min

Lab File: BM011162.D

Acq: 07 Aug 2017 21:07

Instrument :

BNA_M

ClientSampleId :

PL-02-080317-C


Tot Ion:244 Resp: 6200720

Ion Ratio Lower Upper

244 100

212 9.3 4.9 7.3#




122 6.2 6.2 9.4#

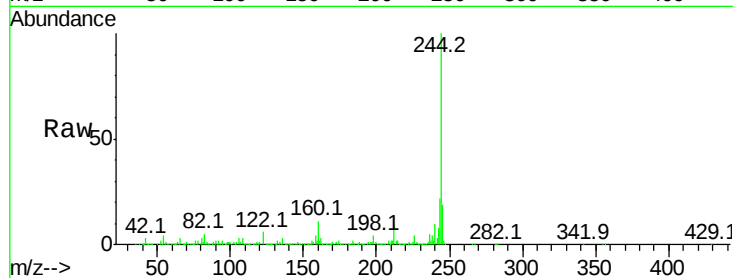

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

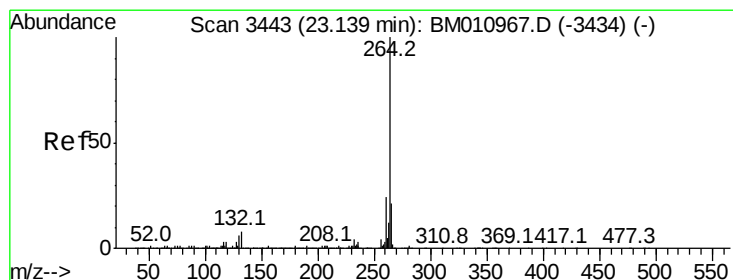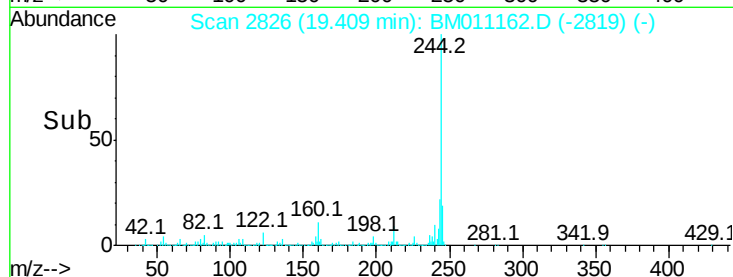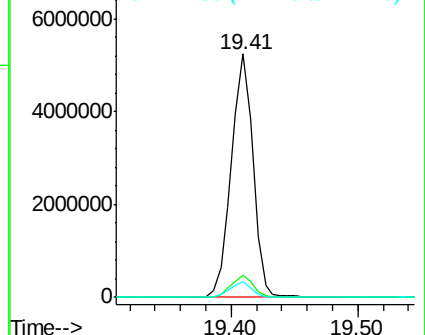

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.05 min Scan# 3445

Delta R.T. -0.09 min

Lab File: BM011162.D

Acq: 07 Aug 2017 21:07


Tgt Ion:264 Resp: 1218972

Ion Ratio Lower Upper

264 100

260 22.4 18.6 27.8

265 20.4 17.3 25.9

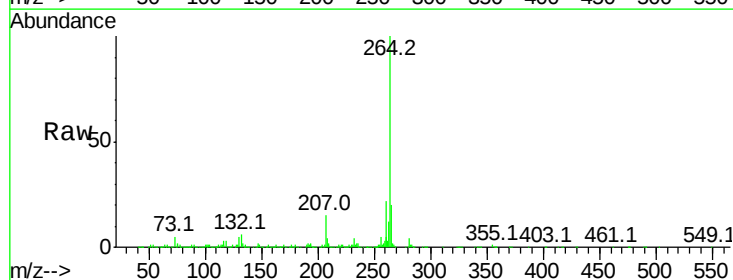

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

