


Data Path : Z:\HPCHEM1\BNA M\Data\BM080717\
 Data File : BM011152.D
 Acq On : 07 Aug 2017 15:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

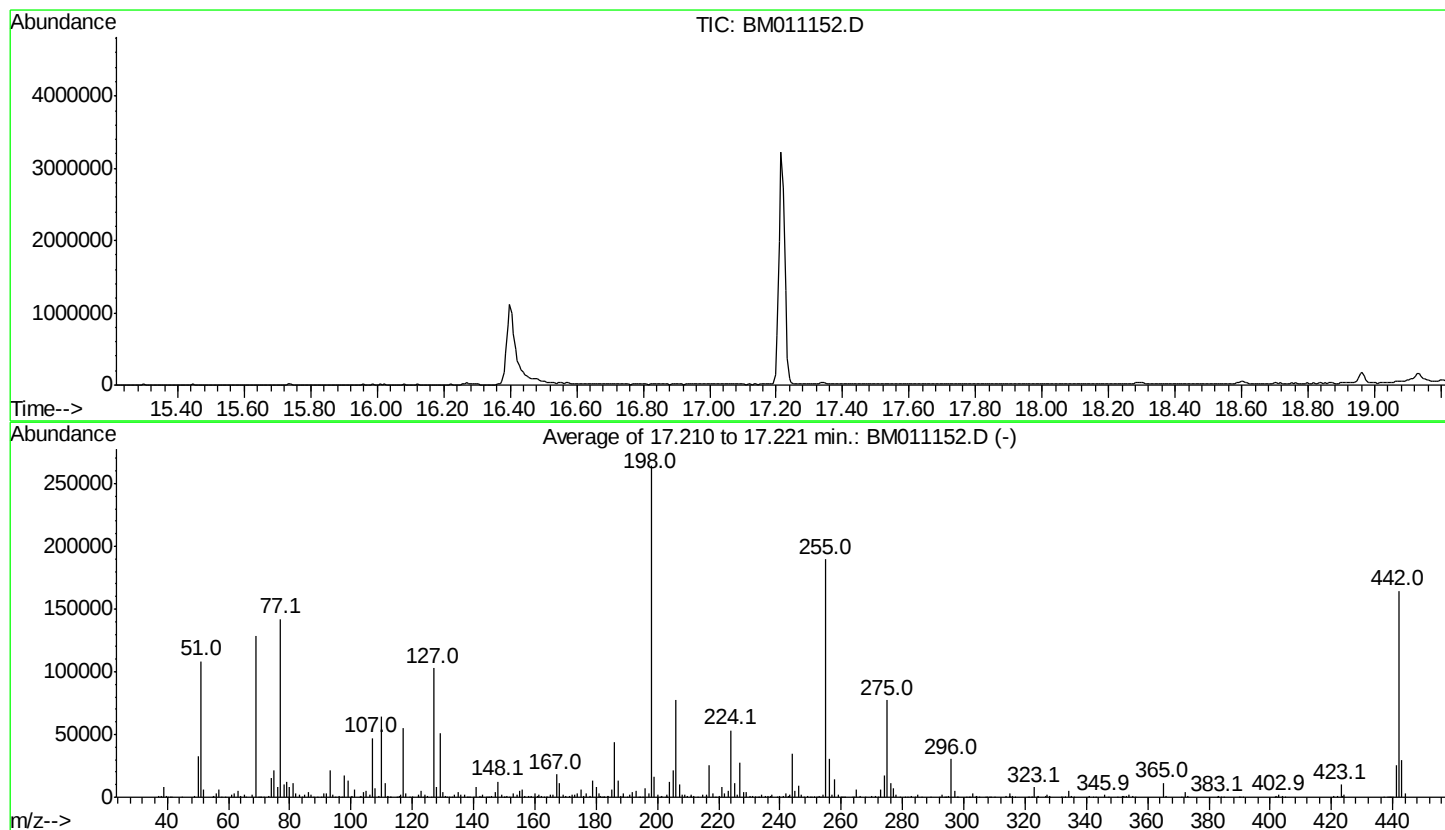

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	108405	PASS
68	69	0.00	2	1.6	2127	PASS
69	198	0.00	100	48.8	128984	PASS
70	69	0.00	2	0.3	401	PASS
127	198	10	80	39.0	102986	PASS
197	198	0.00	2	1.0	2606	PASS
198	198	100	100	100.0	264192	PASS
199	198	5	9	6.3	16654	PASS
275	198	10	60	29.3	77282	PASS
365	198	1	100	4.4	11650	PASS
441	443	0.01	100	84.7	25461	PASS
442	198	50	100	62.2	164341	PASS
443	442	15	24	18.3	30063	PASS