
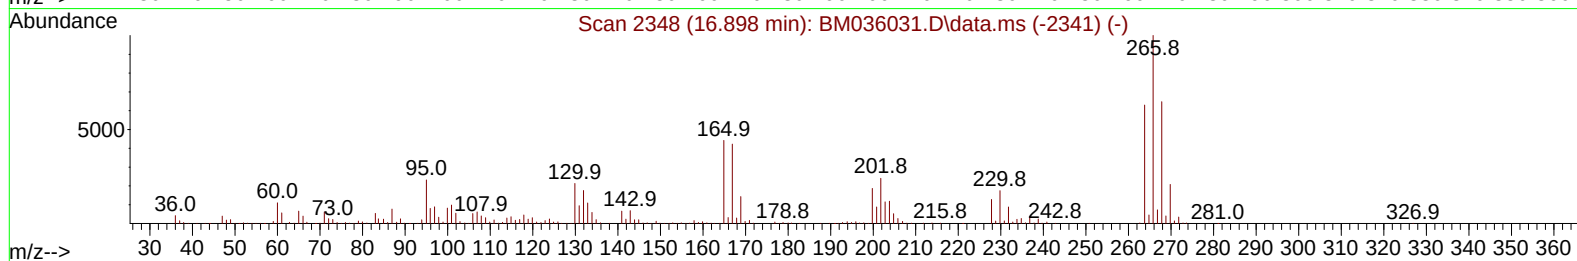
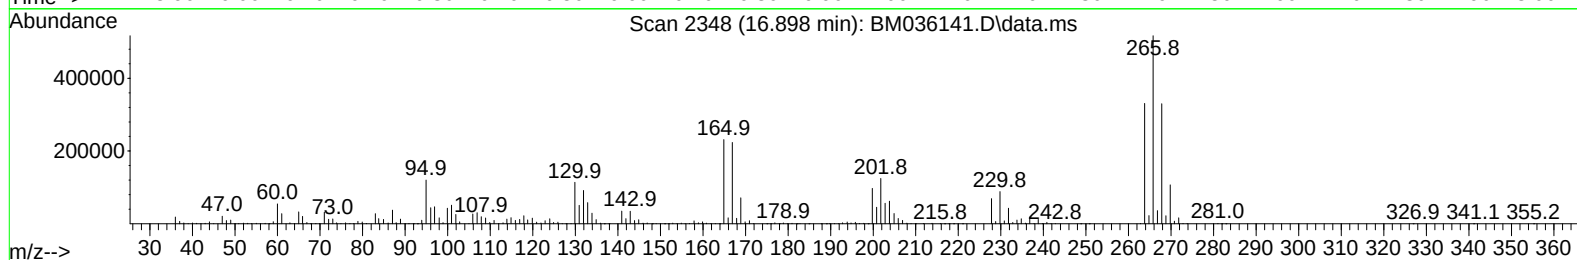


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM080822\  
Data File : BM036141.D  
Acq On : 08 Aug 2022 10:49  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 06:59:15 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM080122.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 08 23:36:56 2022  
Response via : Initial Calibration

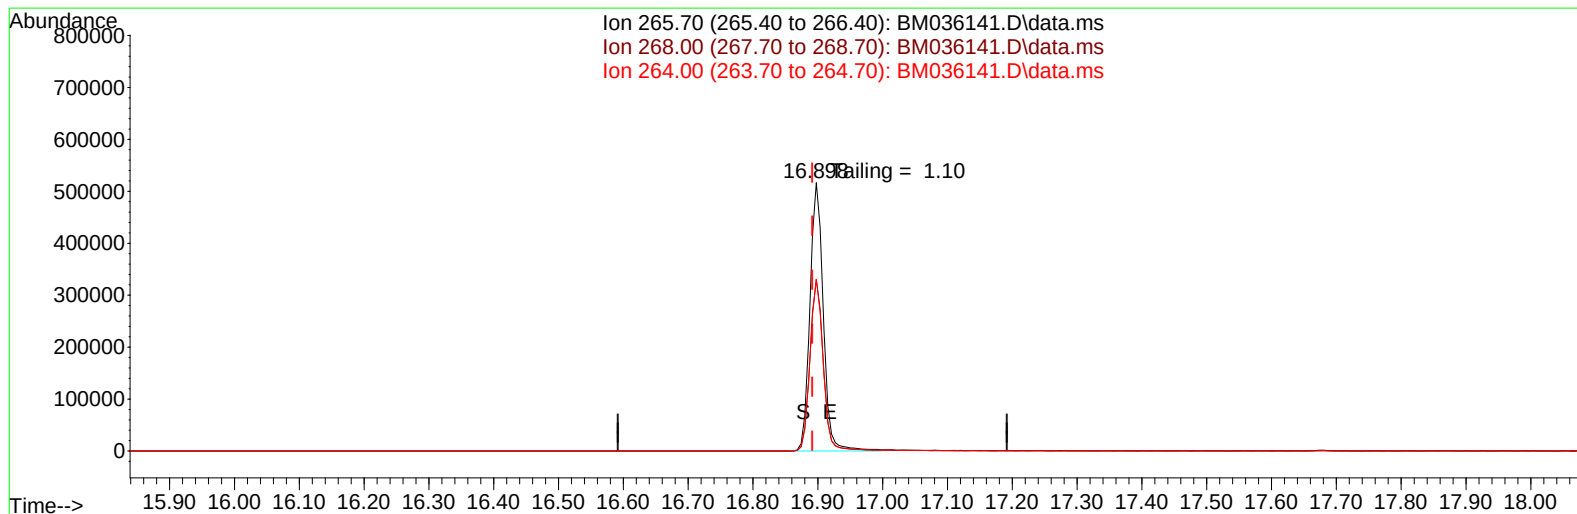

TIC: BM036141.D\data.ms

**(70) Pentachlorophenol (C)**




16.898min (+ 0.006) 239602.40 ng

response 745666

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.90  | 63.87  |
| 264.00 | 63.30  | 64.05  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM080822\  
Data File : BM036141.D  
Acq On : 08 Aug 2022 10:49  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 06:59:15 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM080122.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 08 23:36:56 2022  
Response via : Initial Calibration

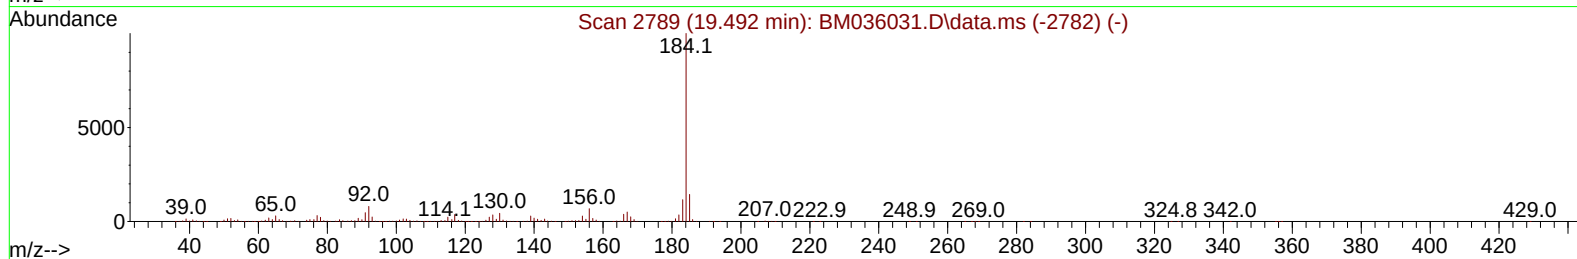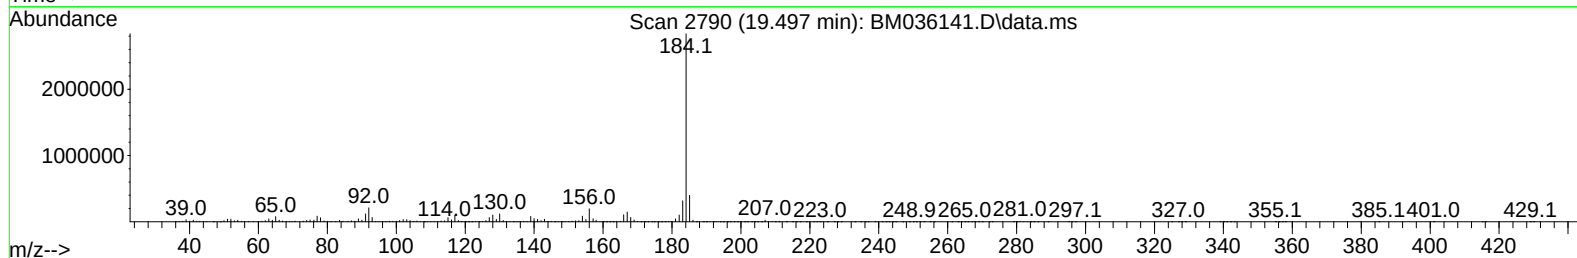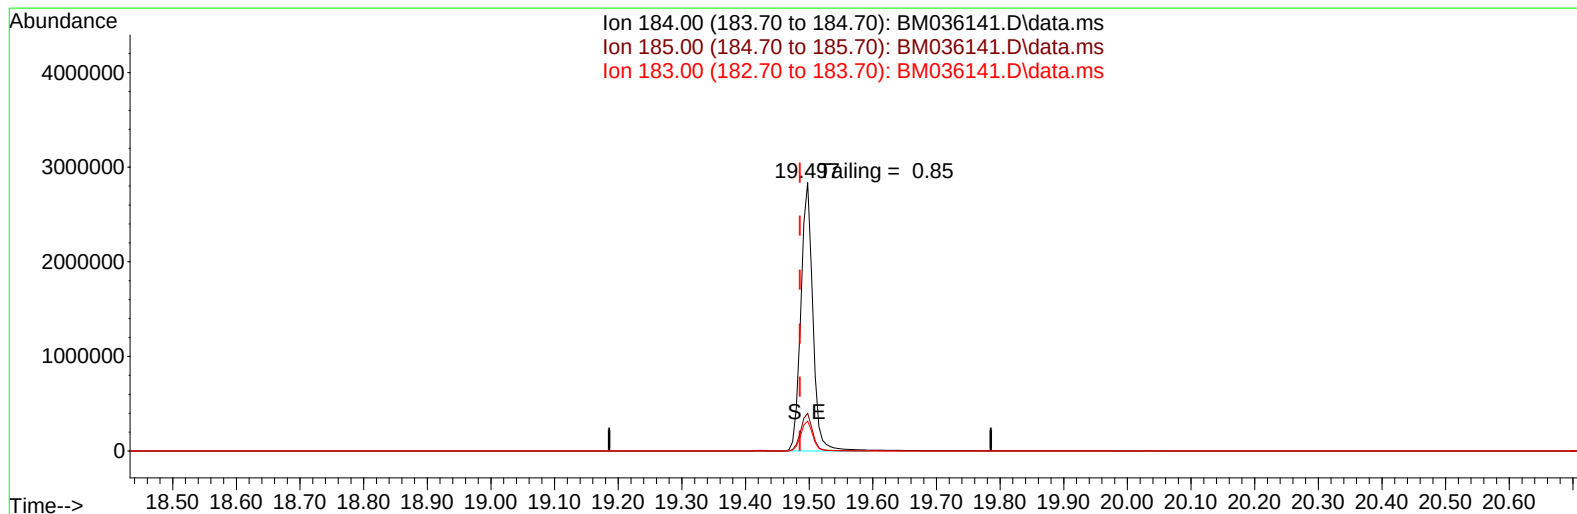

TIC: BM036141.D\data.ms

**(77) Benzidine****19.497min (+ 0.012) 92741.86 ng****response 3746961**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.10  | 14.08  |
| 183.00 | 11.90  | 11.18  |
| 0.00   | 0.00   | 0.00   |