
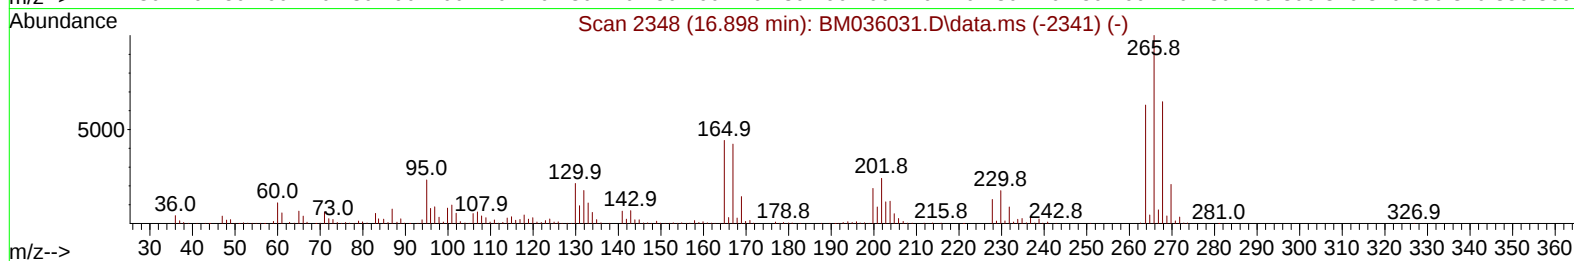
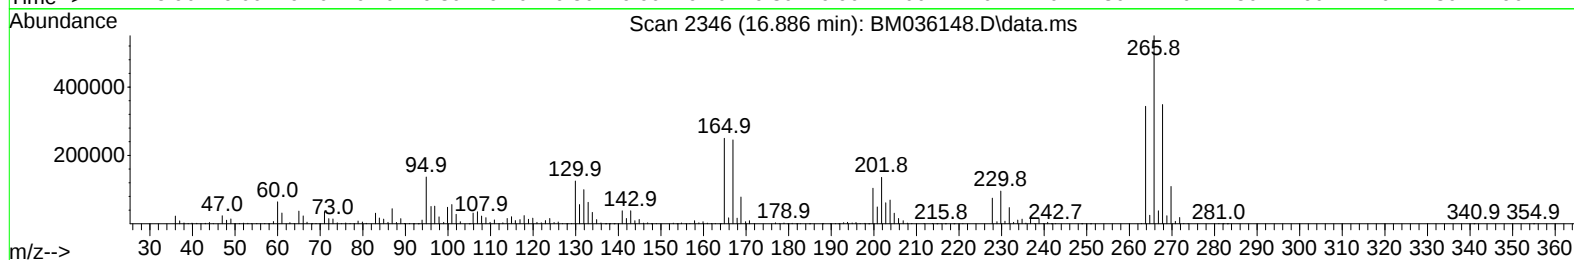


Quant Time: Aug 09 07:00:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 23:36:56 2022
Response via : Initial Calibration

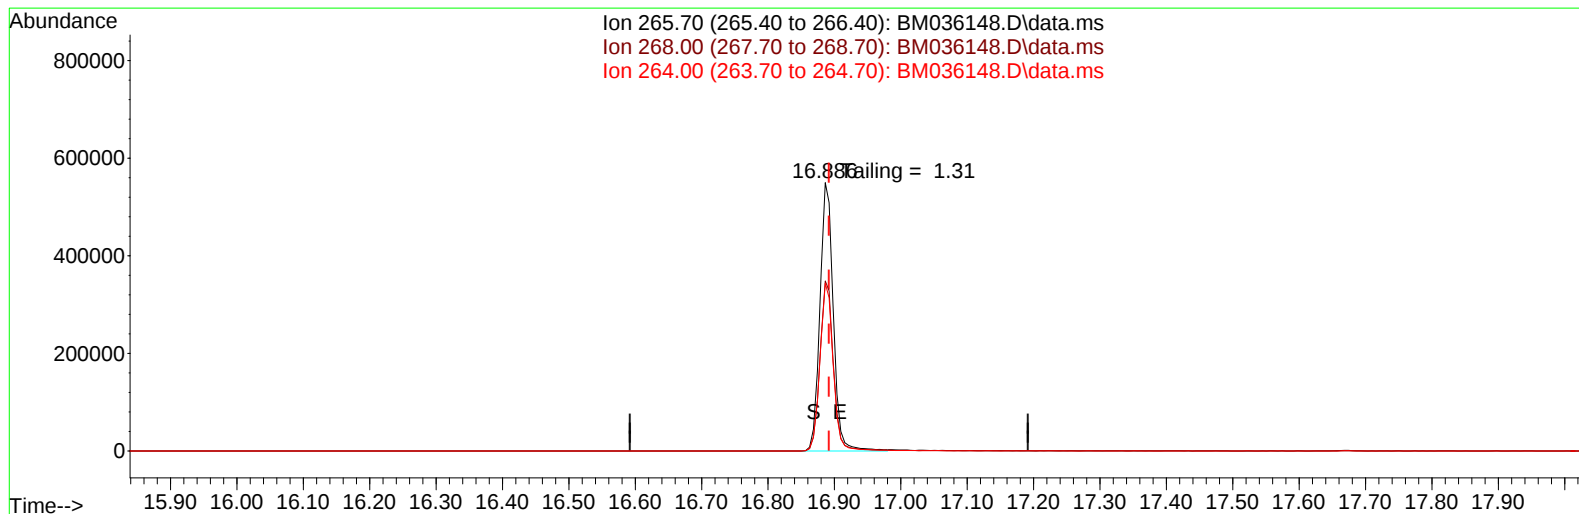

TIC: BM036148.D\data.ms

(70) Pentachlorophenol (C)




16.886min (-0.006) 60247.44 ng

response **775091**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.38
264.00	63.30	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
Data File : BM036148.D
Acq On : 08 Aug 2022 16:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 07:00:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 23:36:56 2022
Response via : Initial Calibration

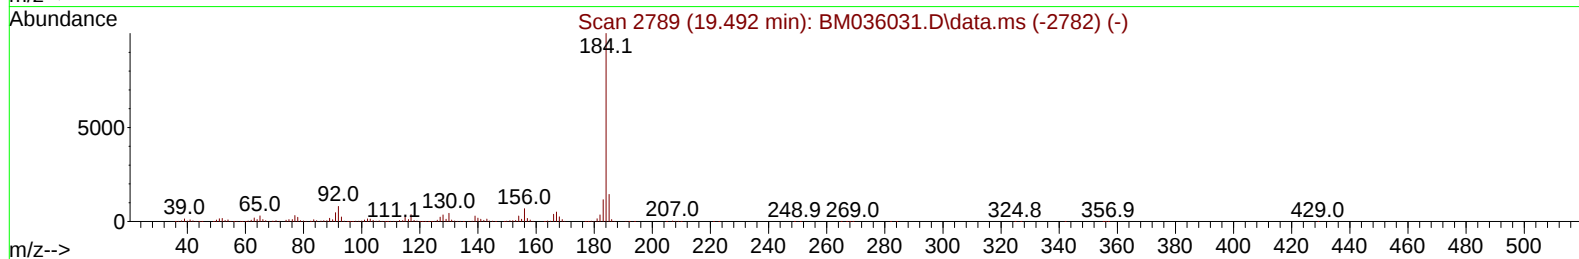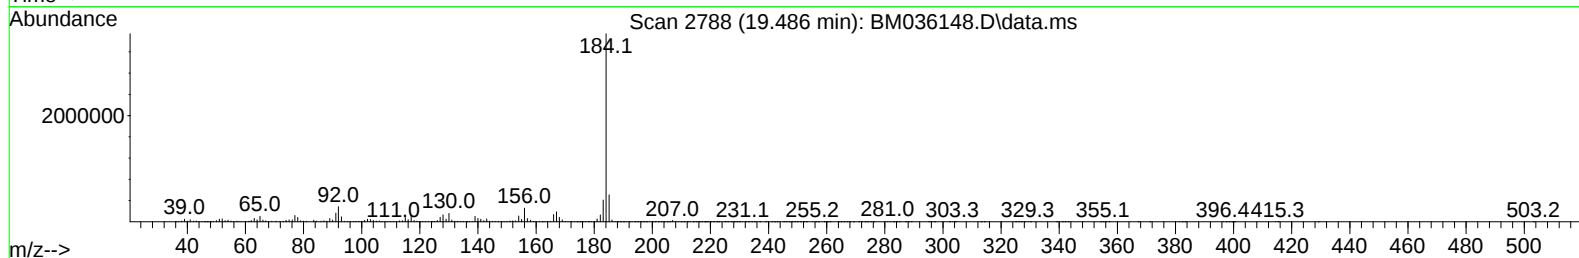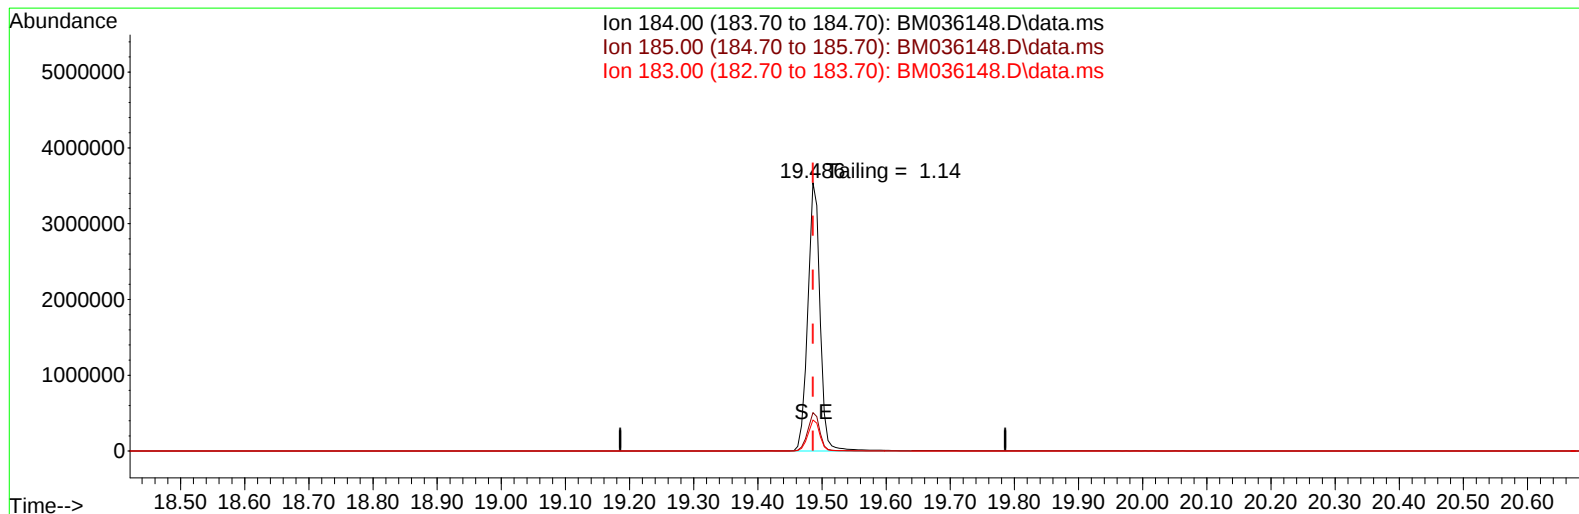

TIC: BM036148.D\data.ms

(77) Benzidine**19.486min (+ 0.000) 64809.00 ng****response 4713927**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.32
183.00	11.90	11.56
0.00	0.00	0.00