

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
 Data File : BM036143.D
 Acq On : 08 Aug 2022 12:03
 Operator : CG/JU
 Sample : PB146780BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146780BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	394	401	420	rBV	5945578	8577136	52.95%	10.817%
2	7.069	669	677	692	rBV	5529006	8731700	53.90%	11.012%
3	7.851	802	810	817	rBV	1126302	1748263	10.79%	2.205%
4	9.022	1000	1009	1024	rBV	3567720	5796965	35.79%	7.311%
5	10.657	1278	1287	1299	rBV	1509431	2525209	15.59%	3.185%
6	13.122	1698	1706	1721	rBV	9202185	13437202	82.95%	16.946%
7	14.498	1932	1940	1953	rBV	2212123	3273511	20.21%	4.128%
8	15.992	2187	2194	2210	rBV	6571263	9311100	57.48%	11.743%
9	17.239	2400	2406	2413	rBV	2585612	3551493	21.92%	4.479%
10	19.868	2847	2853	2868	rBV	13576354	16198630	100.00%	20.429%
11	21.421	3113	3117	3123	rBV	2539124	3090958	19.08%	3.898%
12	23.786	3513	3519	3530	rVB2	1589140	3050828	18.83%	3.848%




Sum of corrected areas: 79292995

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
Data File : BM036143.D
Acq On : 08 Aug 2022 12:03
Operator : CG/JU
Sample : PB146780BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146780BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

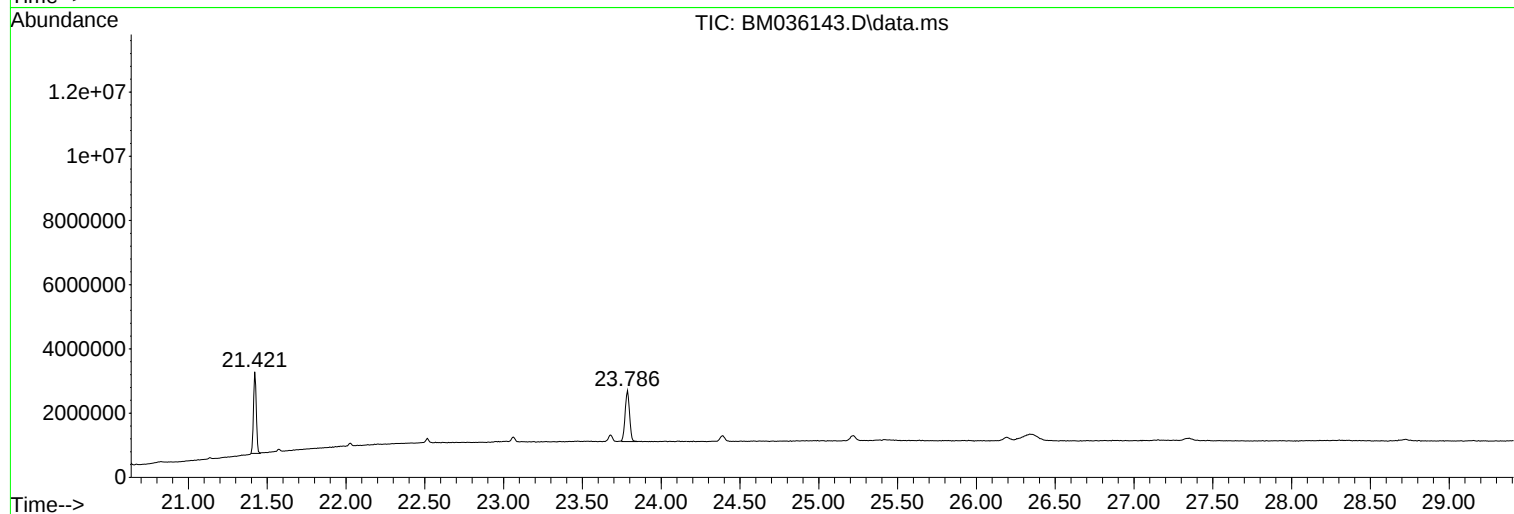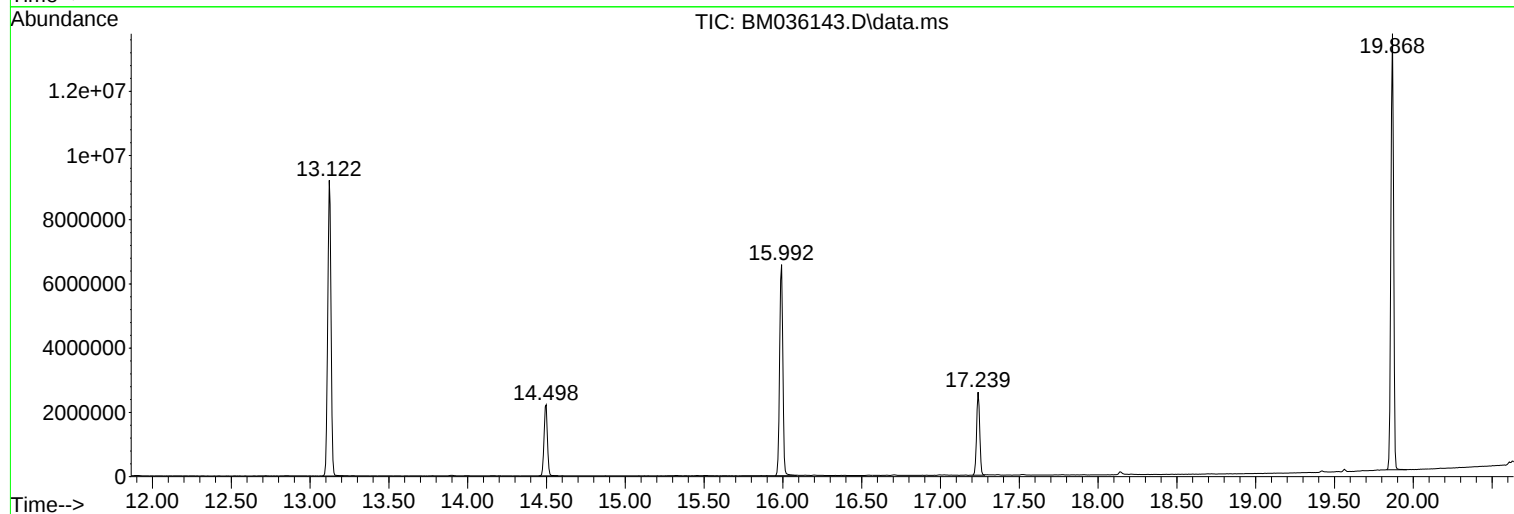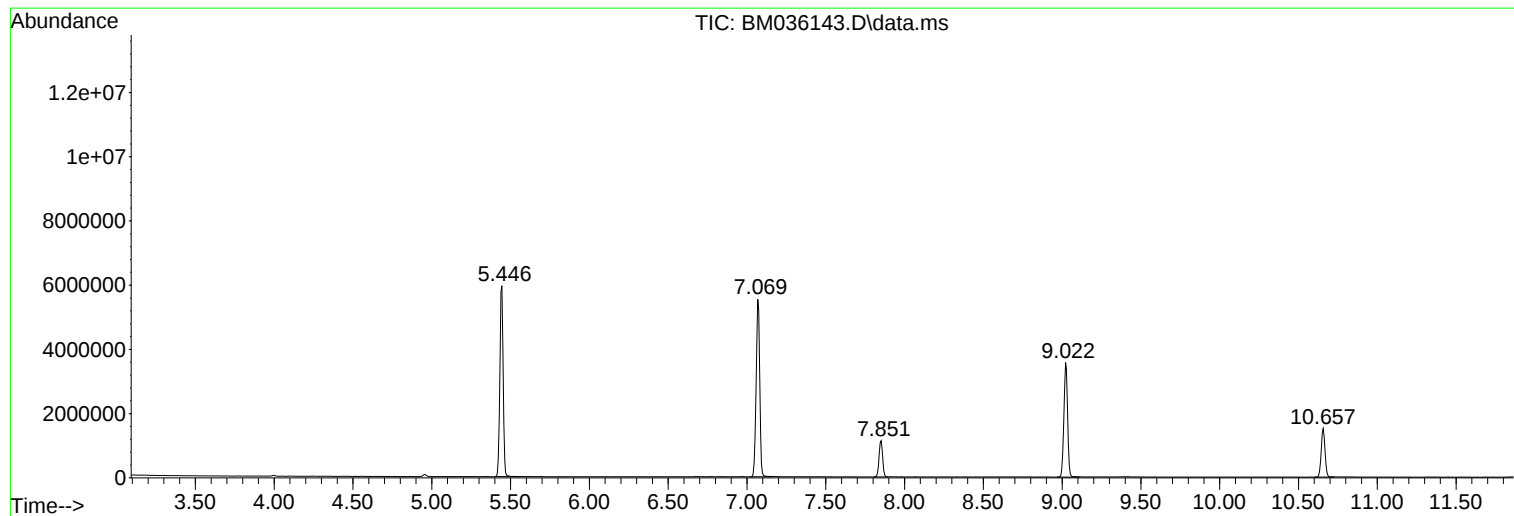

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
Data File : BM036143.D
Acq On : 08 Aug 2022 12:03
Operator : CG/JU
Sample : PB146780BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146780BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
Data File : BM036143.D
Acq On : 08 Aug 2022 12:03
Operator : CG/JU
Sample : PB146780BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146780BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------