

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
 Data File : BM036150.D
 Acq On : 08 Aug 2022 18:40
 Operator : CG/JU
 Sample : PB146776BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146776BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036150.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	392	399	414	rBV	6677003	9365082	43.88%	9.705%
2	7.058	667	675	691	rBV	6119857	9847526	46.14%	10.205%
3	7.846	801	809	821	rBV	1249226	1917611	8.99%	1.987%
4	9.016	999	1008	1020	rBV	3876134	6388359	29.93%	6.620%
5	10.651	1278	1286	1298	rBV	1754164	2867155	13.43%	2.971%
6	13.116	1698	1705	1719	rBV	10454950	15133868	70.91%	15.683%
7	14.486	1931	1938	1950	rBV	2700907	3954574	18.53%	4.098%
8	15.980	2185	2192	2215	rBV	7842539	11473345	53.76%	11.890%
9	17.233	2398	2405	2412	rBV	3347844	4660783	21.84%	4.830%
10	19.557	2796	2800	2804	rBV	325351	358088	1.68%	0.371%
11	19.863	2845	2852	2857	rBV	16672370	21341272	100.00%	22.116%
12	20.604	2974	2978	2985	rBV2	229320	379541	1.78%	0.393%
13	21.415	3111	3116	3124	rBV	3613936	4602928	21.57%	4.770%
14	23.768	3510	3516	3527	rVB2	2166250	4208250	19.72%	4.361%




Sum of corrected areas: 96498382

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
Data File : BM036150.D
Acq On : 08 Aug 2022 18:40
Operator : CG/JU
Sample : PB146776BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146776BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

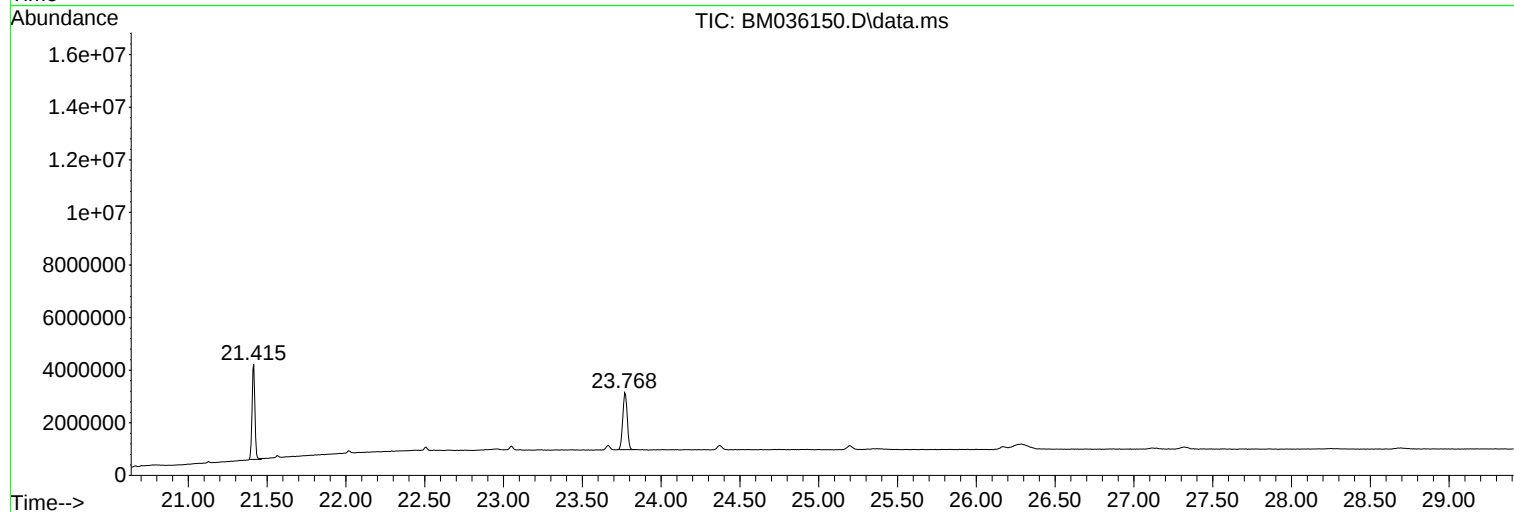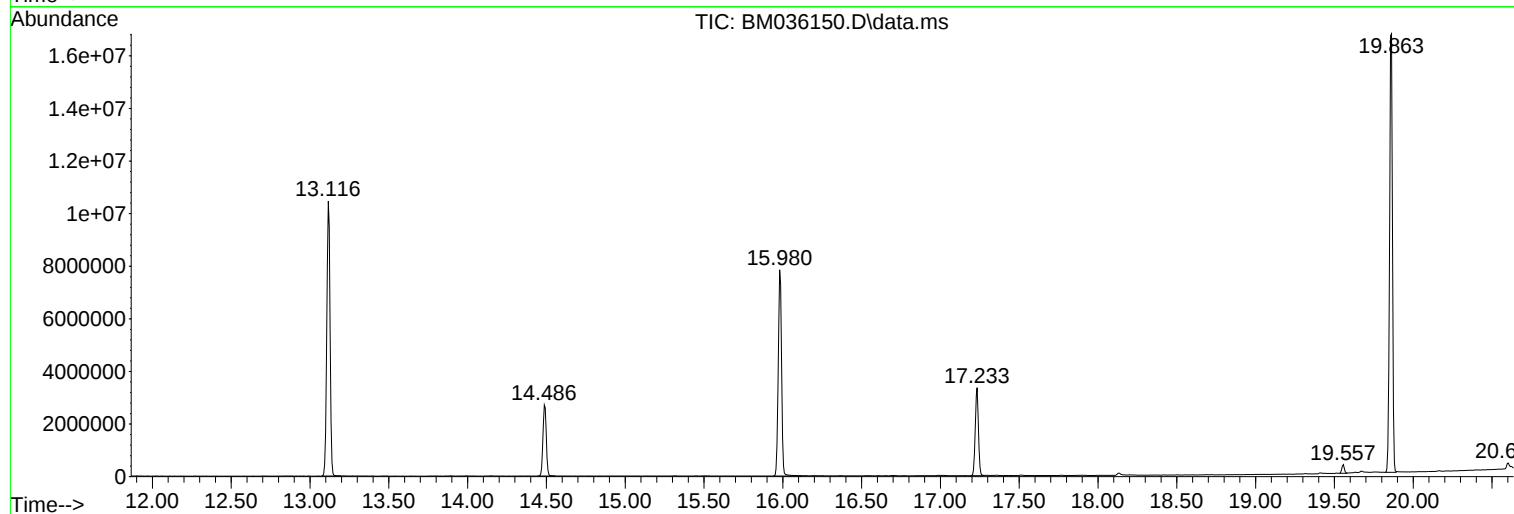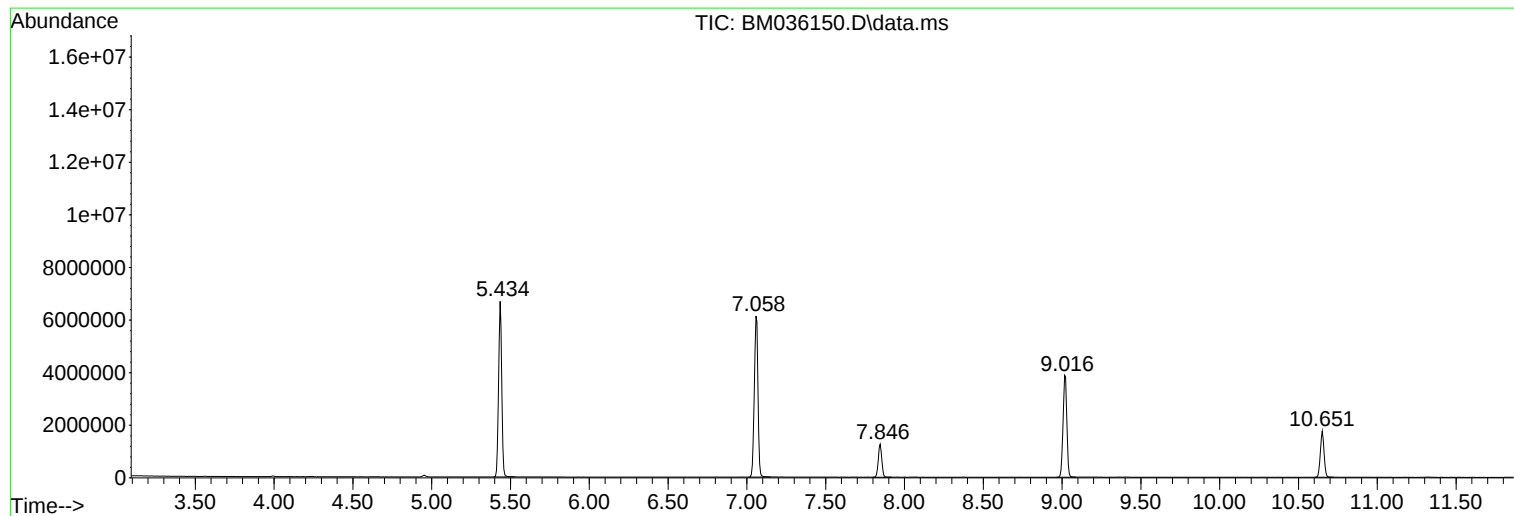

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
Data File : BM036150.D
Acq On : 08 Aug 2022 18:40
Operator : CG/JU
Sample : PB146776BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146776BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
Data File : BM036150.D
Acq On : 08 Aug 2022 18:40
Operator : CG/JU
Sample : PB146776BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146776BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------