
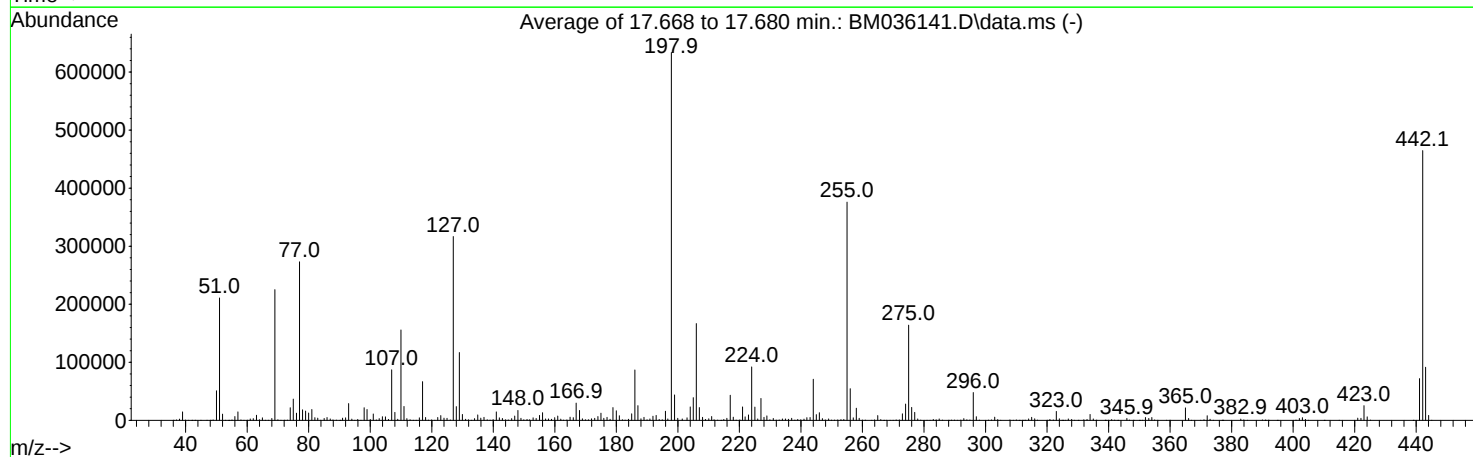


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
 Data File : BM036141.D
 Acq On : 08 Aug 2022 10:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 10 22:19:26 2022

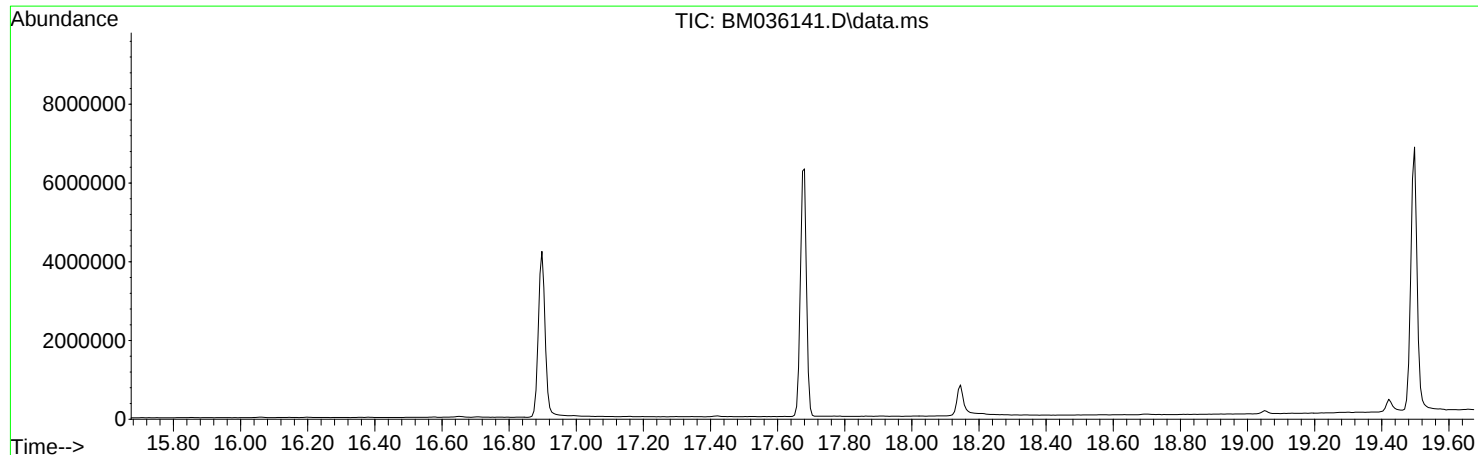




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	210826	PASS
68	69	0.00	2	1.5	3341	PASS
69	198	0.00	100	35.5	225197	PASS
70	69	0.00	2	0.5	1152	PASS
127	198	10	80	50.0	316596	PASS
197	198	0.00	2	0.4	2611	PASS
198	198	100	100	100.0	633707	PASS
199	198	5	9	6.9	43779	PASS
275	198	10	60	25.9	164061	PASS
365	198	1	100	3.4	21661	PASS
441	198	0.01	100	11.3	71901	PASS
442	442	50	100	100.0	464811	PASS
443	442	15	24	19.7	91403	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
 Data File : BM036141.D
 Acq On : 08 Aug 2022 10:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 09 06:59:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 23:36:56 2022
 Response via : Initial Calibration

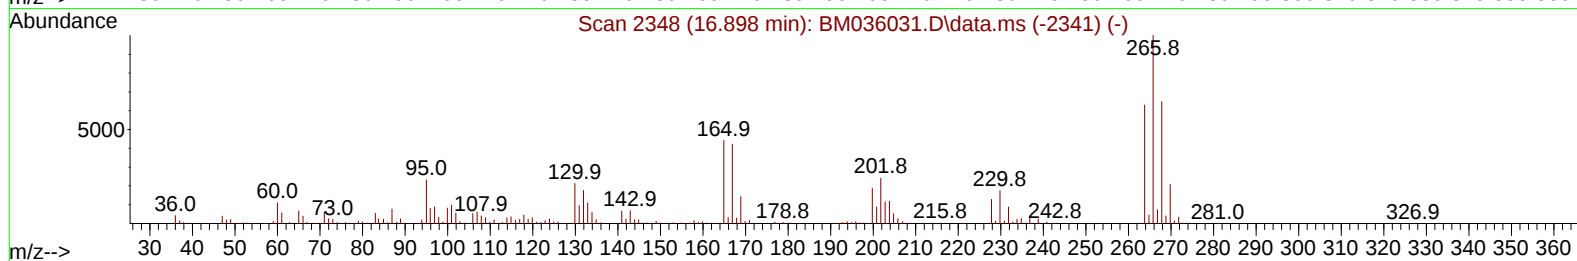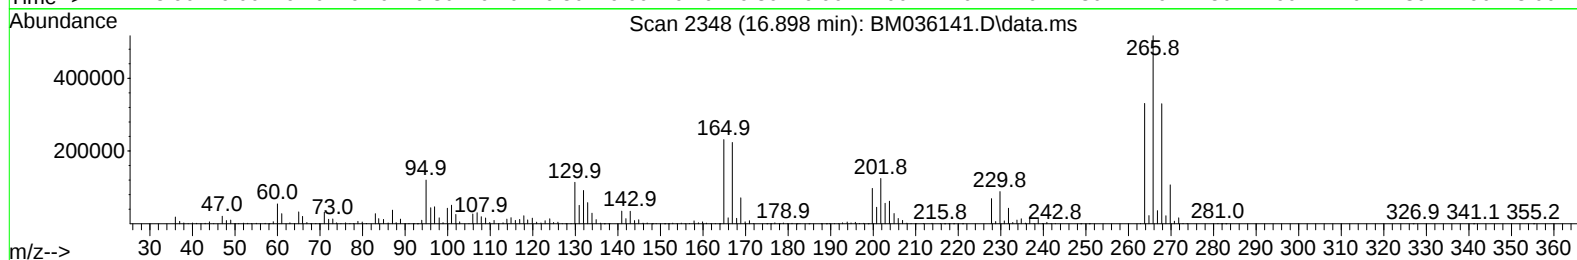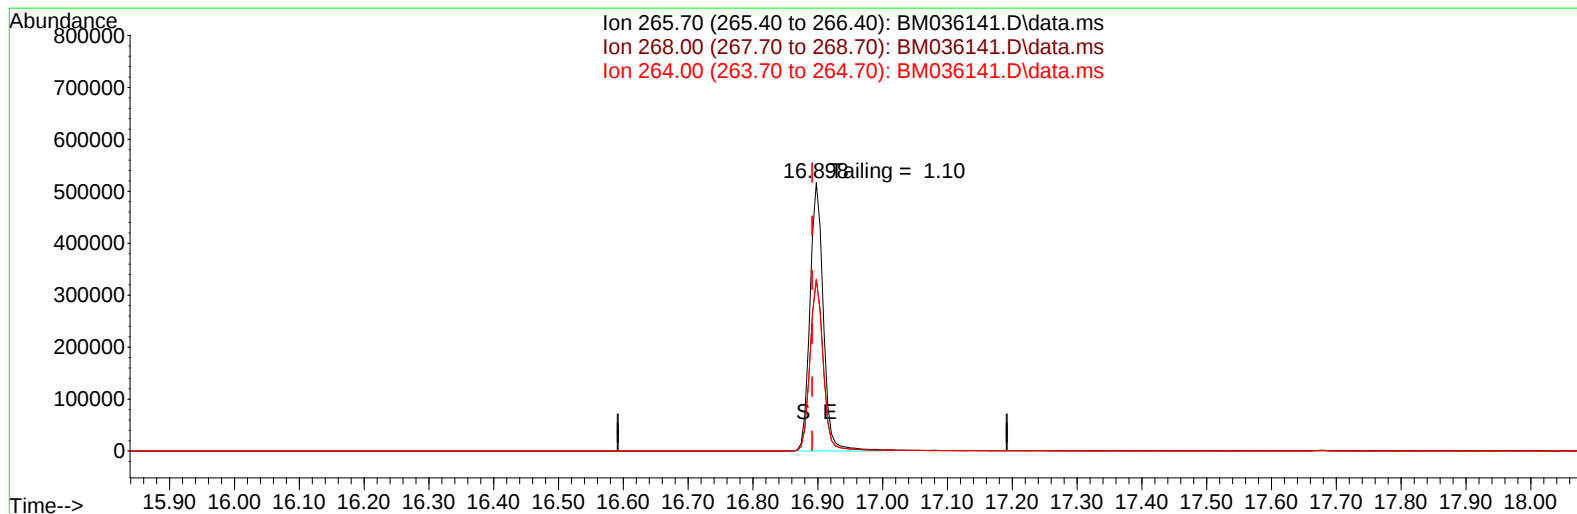

TIC: BM036141.D\data.ms

(70) Pentachlorophenol (C)

16.898min (+ 0.006) 239602.40 ng




response 745666

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.87
264.00	63.30	64.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
Data File : BM036141.D
Acq On : 08 Aug 2022 10:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 09 06:59:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 23:36:56 2022
Response via : Initial Calibration

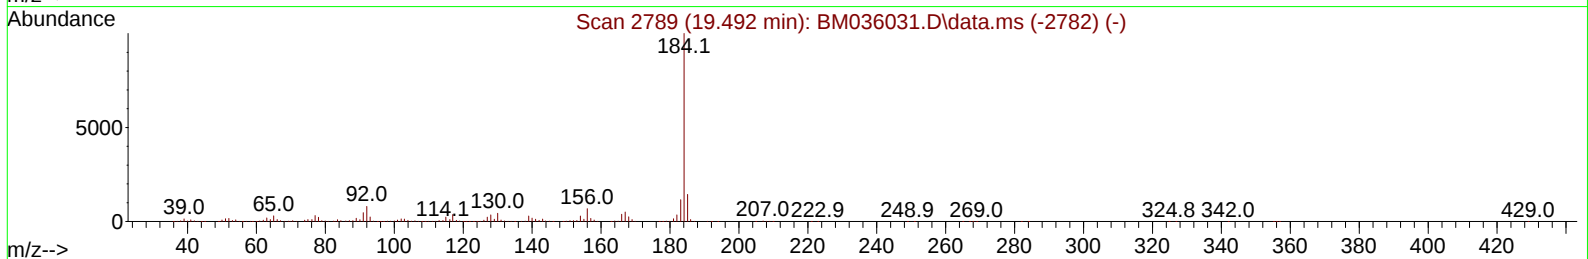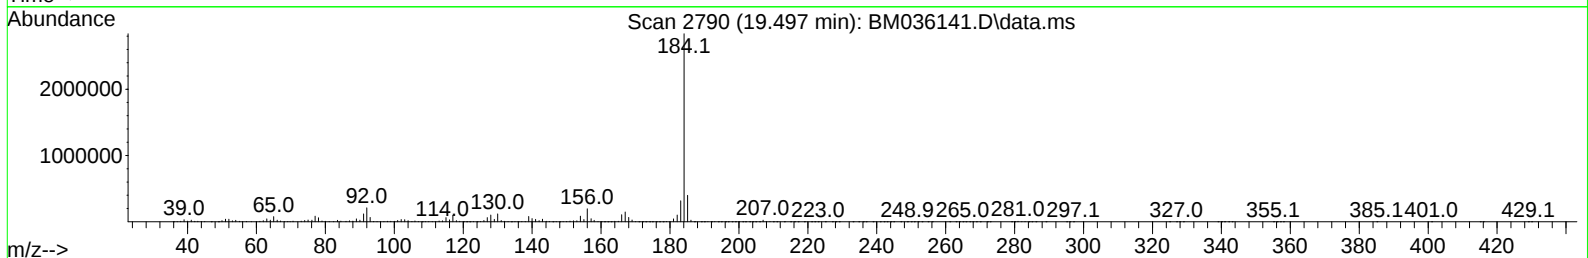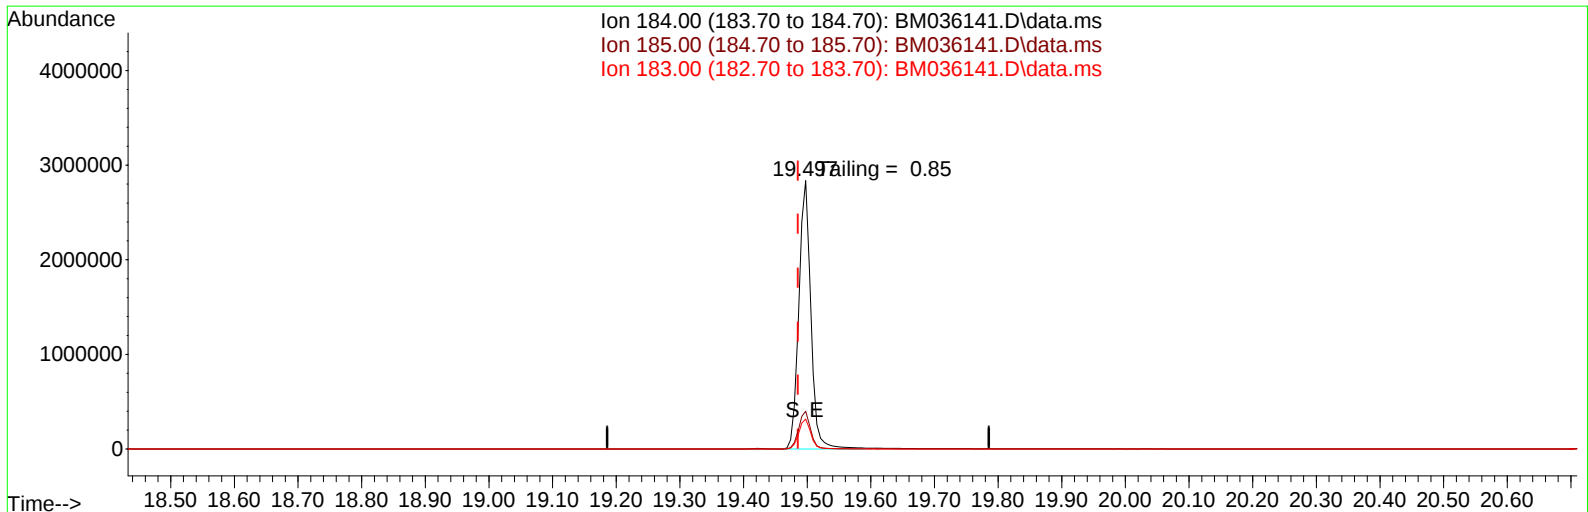

TIC: BM036141.D\data.ms

(77) Benzidine

19.497min (+ 0.012) 92741.86 ng

response 3746961

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.08
183.00	11.90	11.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/8/2022	BNA_M	<u>BM036141.D</u>
Compound Name	Response	Retention Time
DDT	2083743	20.721
DDD	25984	20.286
DDE	2348	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28332	2112075	1.34

Instrument :
BNA_M
ClientSampleId :
DFTPP