


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
 Data File : BM036148.D
 Acq On : 08 Aug 2022 16:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 10 22:19:26 2022

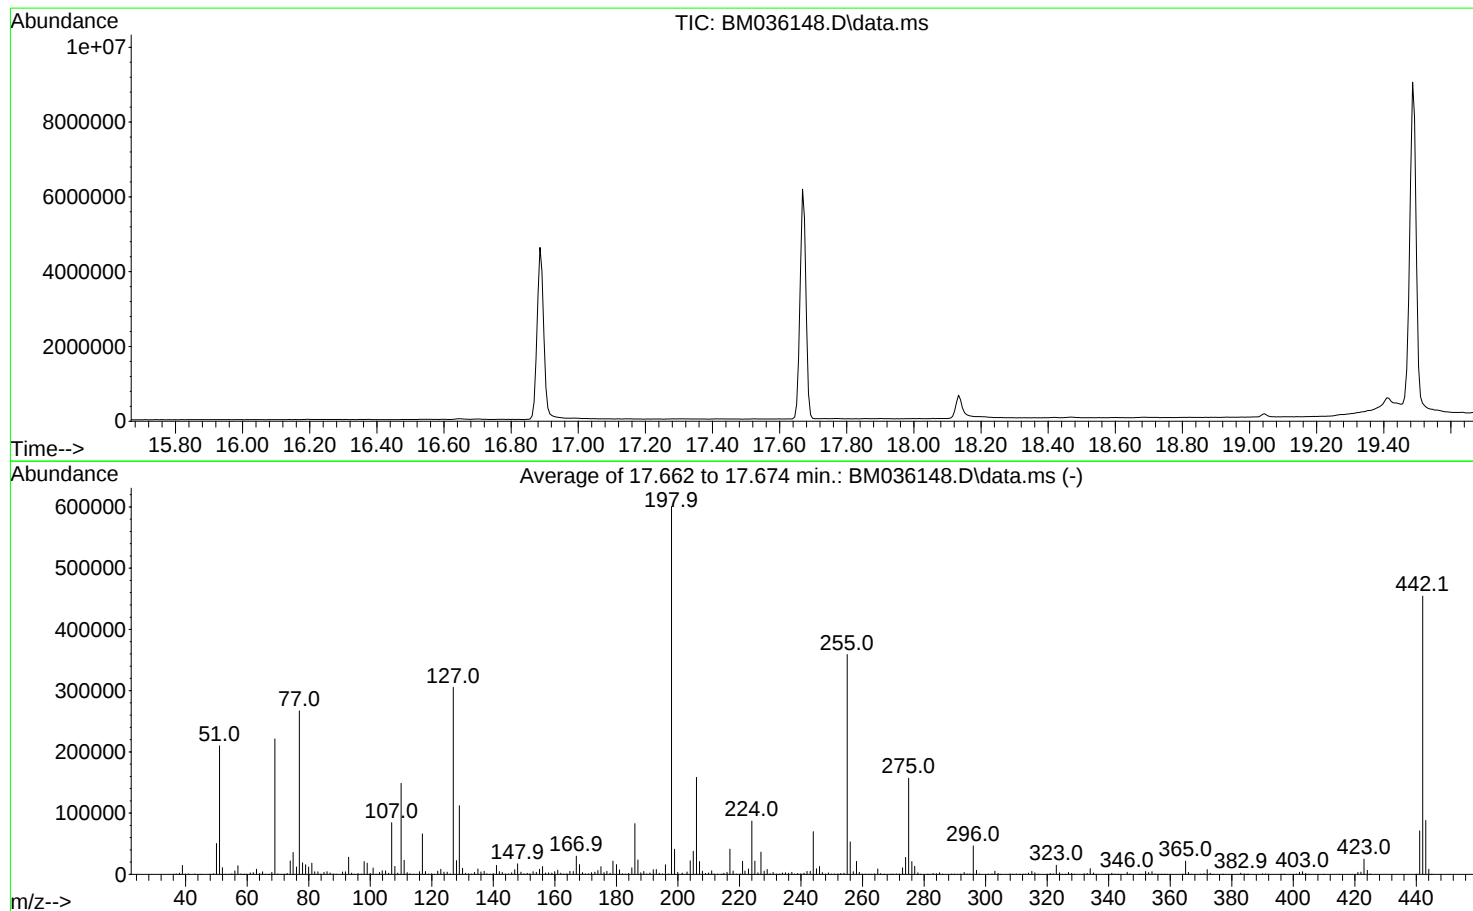




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	209817	PASS
68	69	0.00	2	1.5	3308	PASS
69	198	0.00	100	36.8	221263	PASS
70	69	0.00	2	0.4	833	PASS
127	198	10	80	50.8	305387	PASS
197	198	0.00	2	0.1	512	PASS
198	198	100	100	100.0	600704	PASS
199	198	5	9	6.8	41139	PASS
275	198	10	60	26.1	157067	PASS
365	198	1	100	3.6	21712	PASS
441	198	0.01	100	11.8	71013	PASS
442	442	50	100	100.0	454336	PASS
443	442	15	24	19.4	87976	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\  
Data File : BM036148.D  
Acq On    : 08 Aug 2022  16:46  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 09 07:00:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 23:36:56 2022
Response via : Initial Calibration

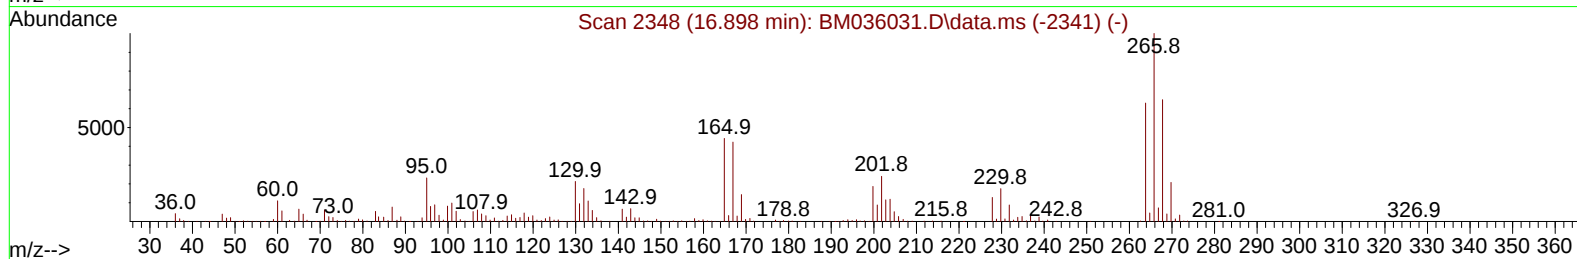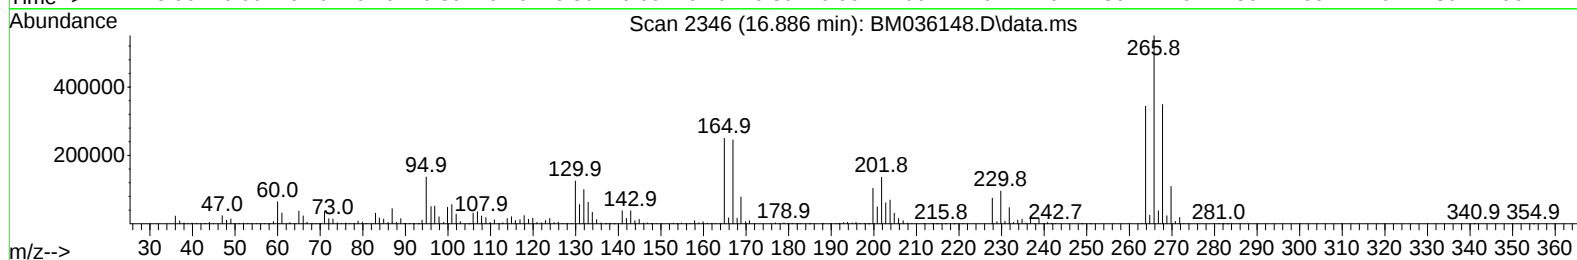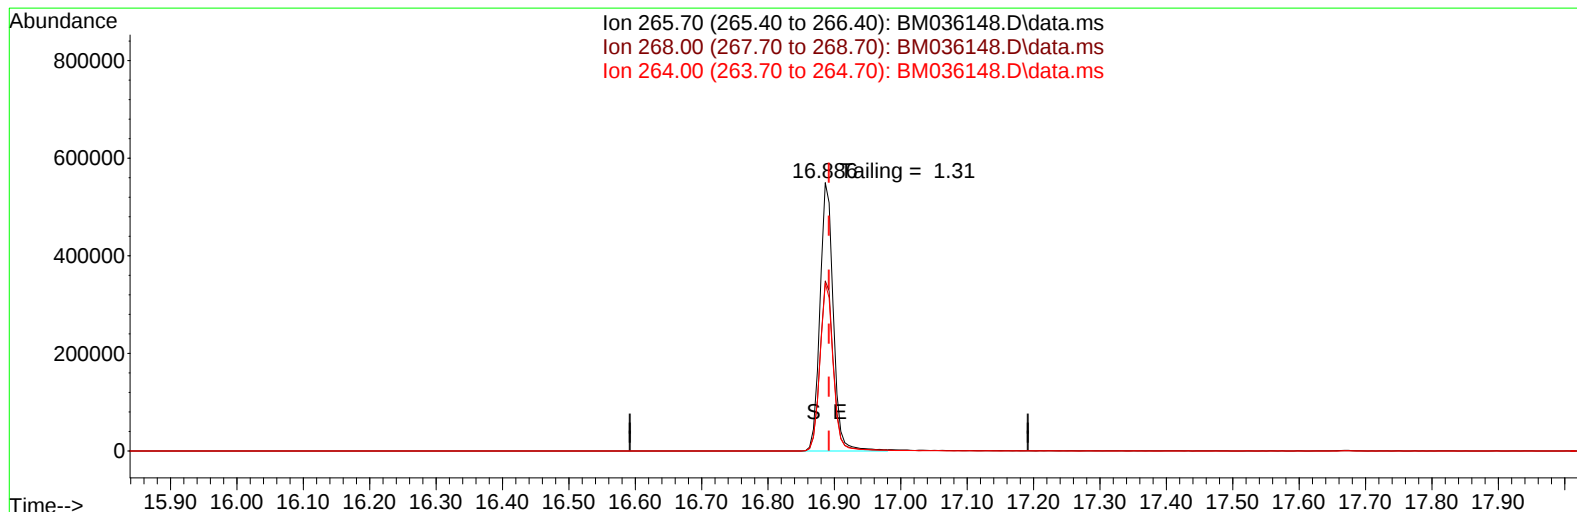

TIC: BM036148.D\data.ms

(70) Pentachlorophenol (C)

16.886min (-0.006) 60247.44 ng




response **775091**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.38
264.00	63.30	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080822\
 Data File : BM036148.D
 Acq On : 08 Aug 2022 16:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 09 07:00:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 23:36:56 2022
 Response via : Initial Calibration

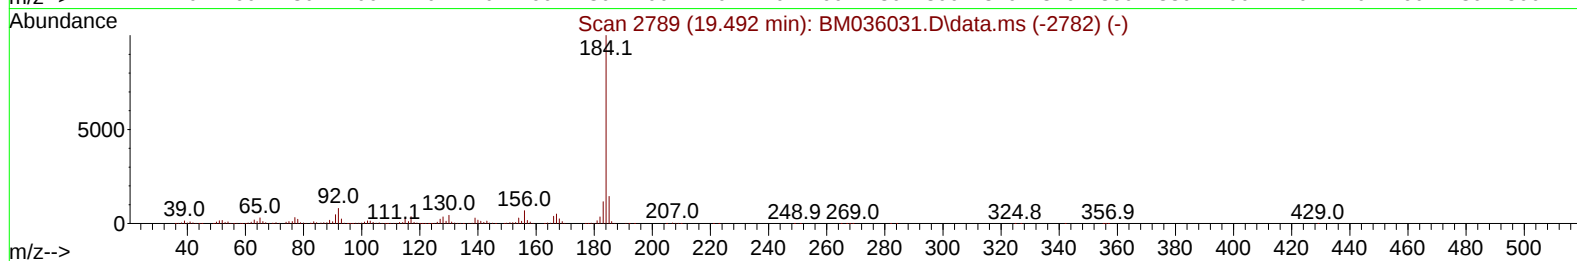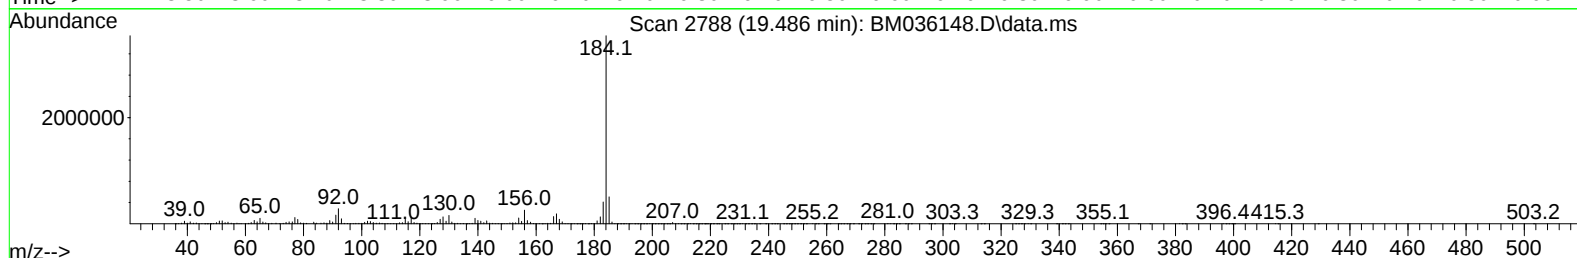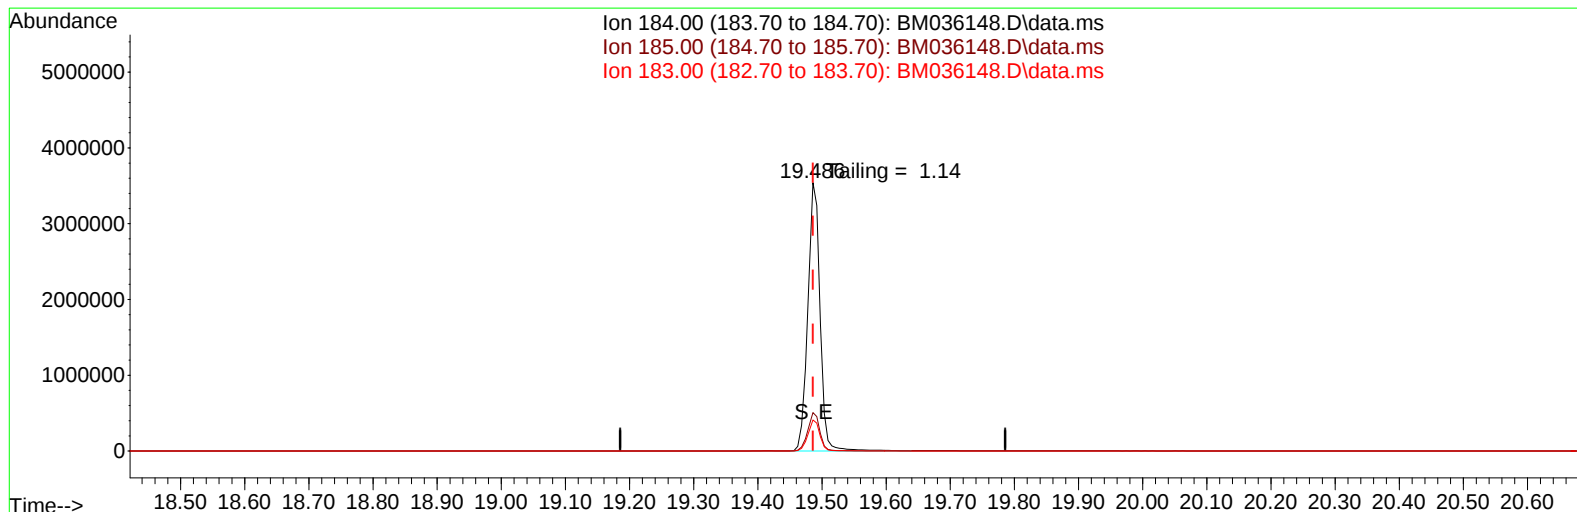

TIC: BM036148.D\data.ms

(77) Benzidine**19.486min (+ 0.000) 64809.00 ng****response 4713927**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.32
183.00	11.90	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/8/2022	BNA_M	<u>BM036148.D</u>
Compound Name	Response	Retention Time
DDT	2301834	20.715
DDD	28888	20.274
DDE	2501	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31389	2333223	1.35

Instrument :
BNA_M
ClientSampleId :
DFTPP