
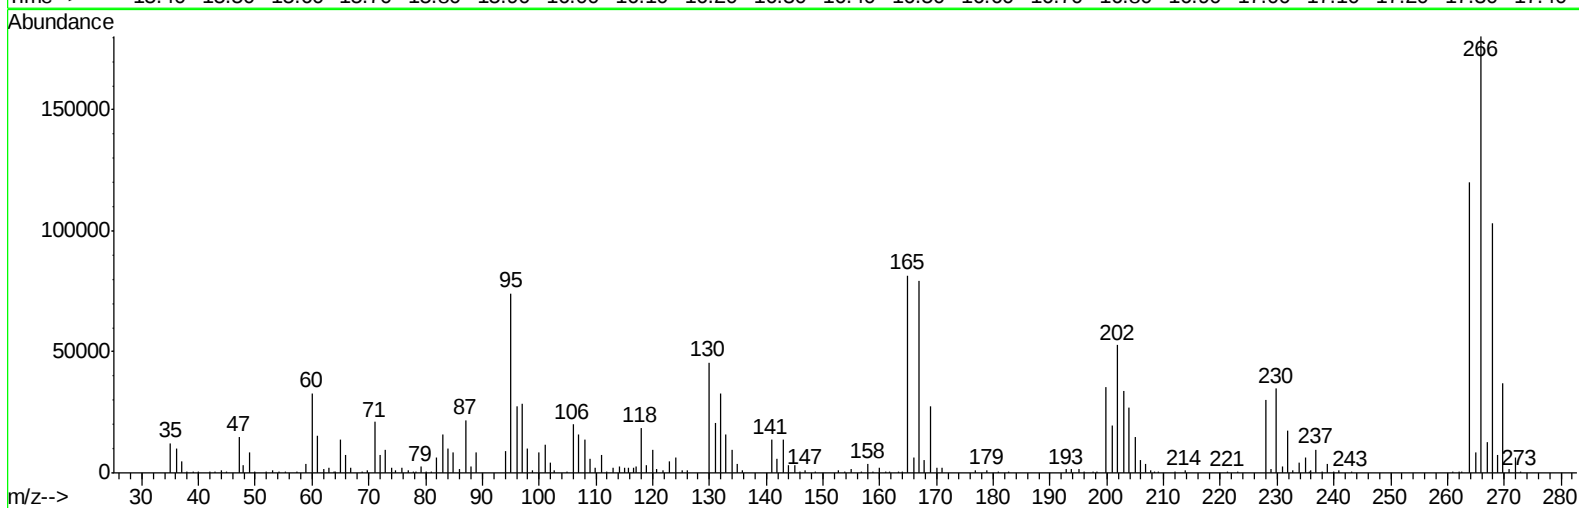


Data Path : Z:\HPCHEM1\BNA M\DATA\BM080917\
Data File : BM011189.D
Acq On : 09 Aug 2017 23:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 03:56:52 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

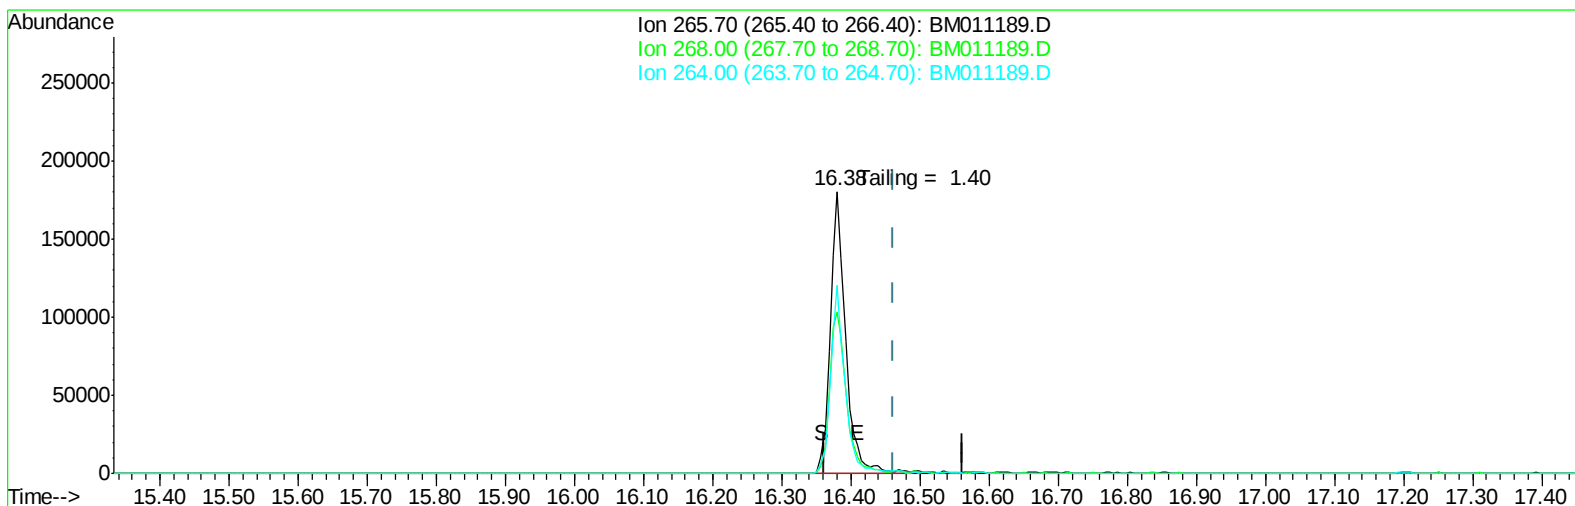

TIC: BM011189.D

(69) Pentachlorophenol (C)



16.380min (-0.082) 245726.40ng

response 274213

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	57.26
264.00	61.20	66.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080917\
Data File : BM011189.D
Acq On : 09 Aug 2017 23:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 03:56:52 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

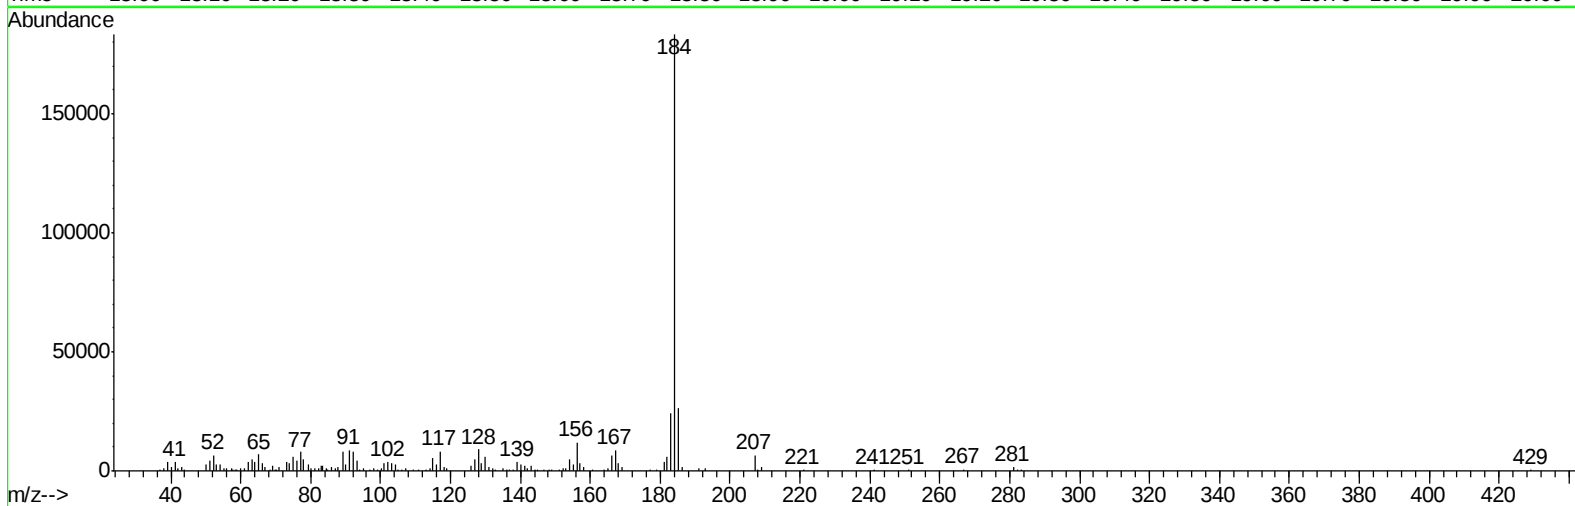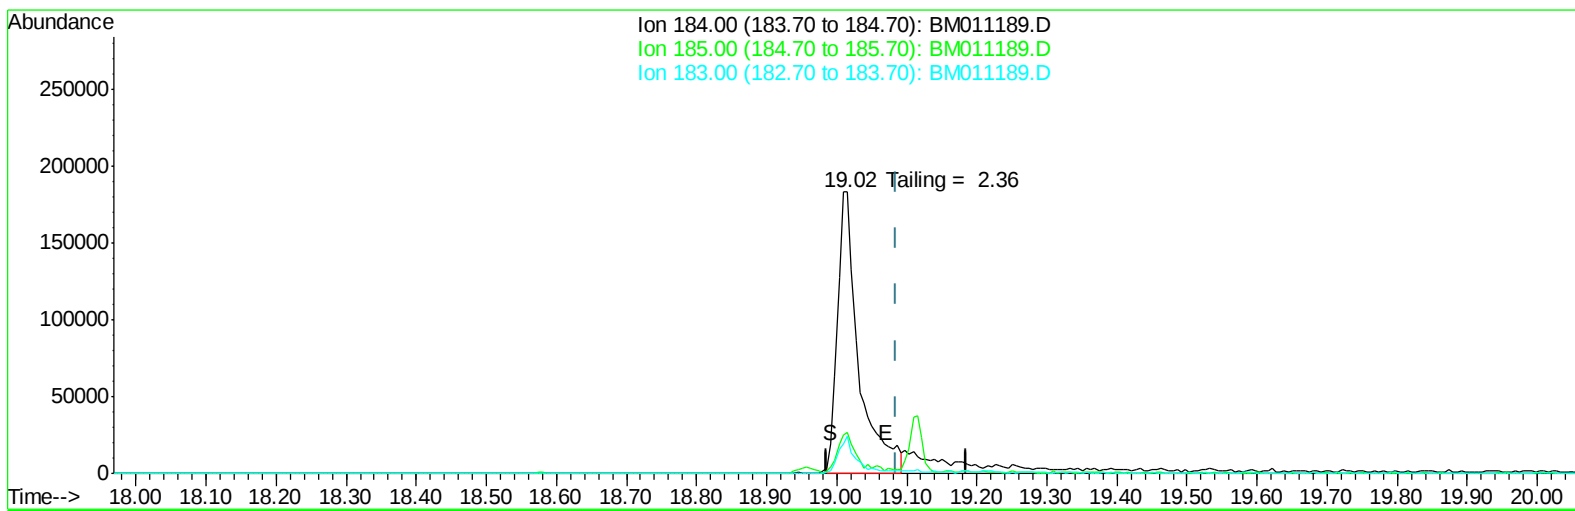

TIC: BM011189.D

(76) Benzidine

19.015min (-0.071) 67222.73ng m

response 385957

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.34
183.00	11.10	13.28
0.00	0.00	0.00