


Data Path : Z:\HPCHEM1\BNA M\Data\BM080917\
 Data File : BM011172.D
 Acq On : 09 Aug 2017 13:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

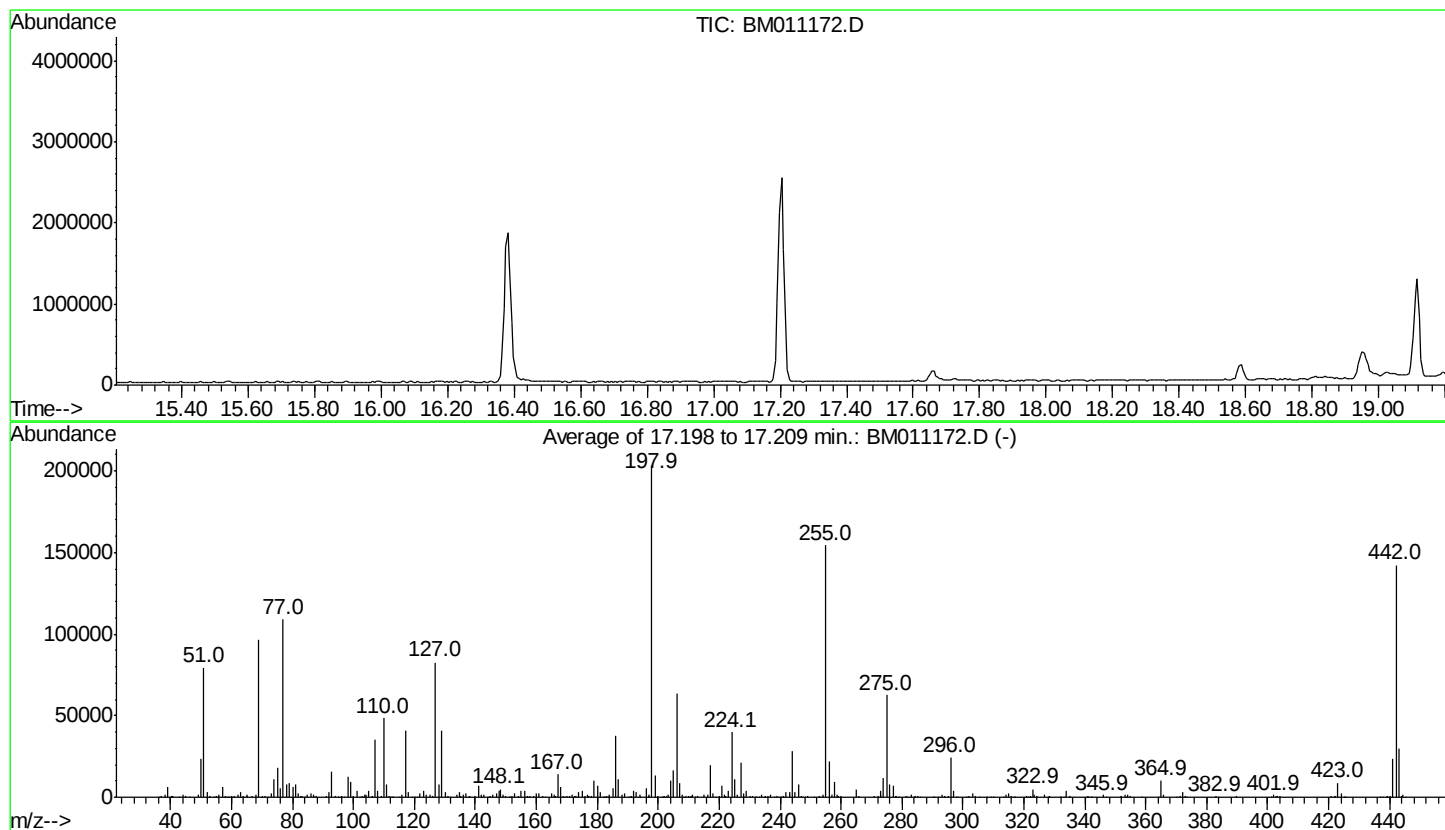

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	79596	PASS
68	69	0.00	2	1.9	1796	PASS
69	198	0.00	100	47.7	96909	PASS
70	69	0.00	2	0.9	829	PASS
127	198	10	80	40.6	82549	PASS
197	198	0.00	2	0.6	1244	PASS
198	198	100	100	100.0	203285	PASS
199	198	5	9	6.7	13710	PASS
275	198	10	60	30.7	62421	PASS
365	198	1	100	4.9	10057	PASS
441	443	0.01	100	77.6	23440	PASS
442	198	50	100	70.0	142221	PASS
443	442	15	24	21.2	30208	PASS