


Data Path : Z:\HPCHEM1\BNA M\Data\BM080917\
 Data File : BM011189.D
 Acq On : 09 Aug 2017 23:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

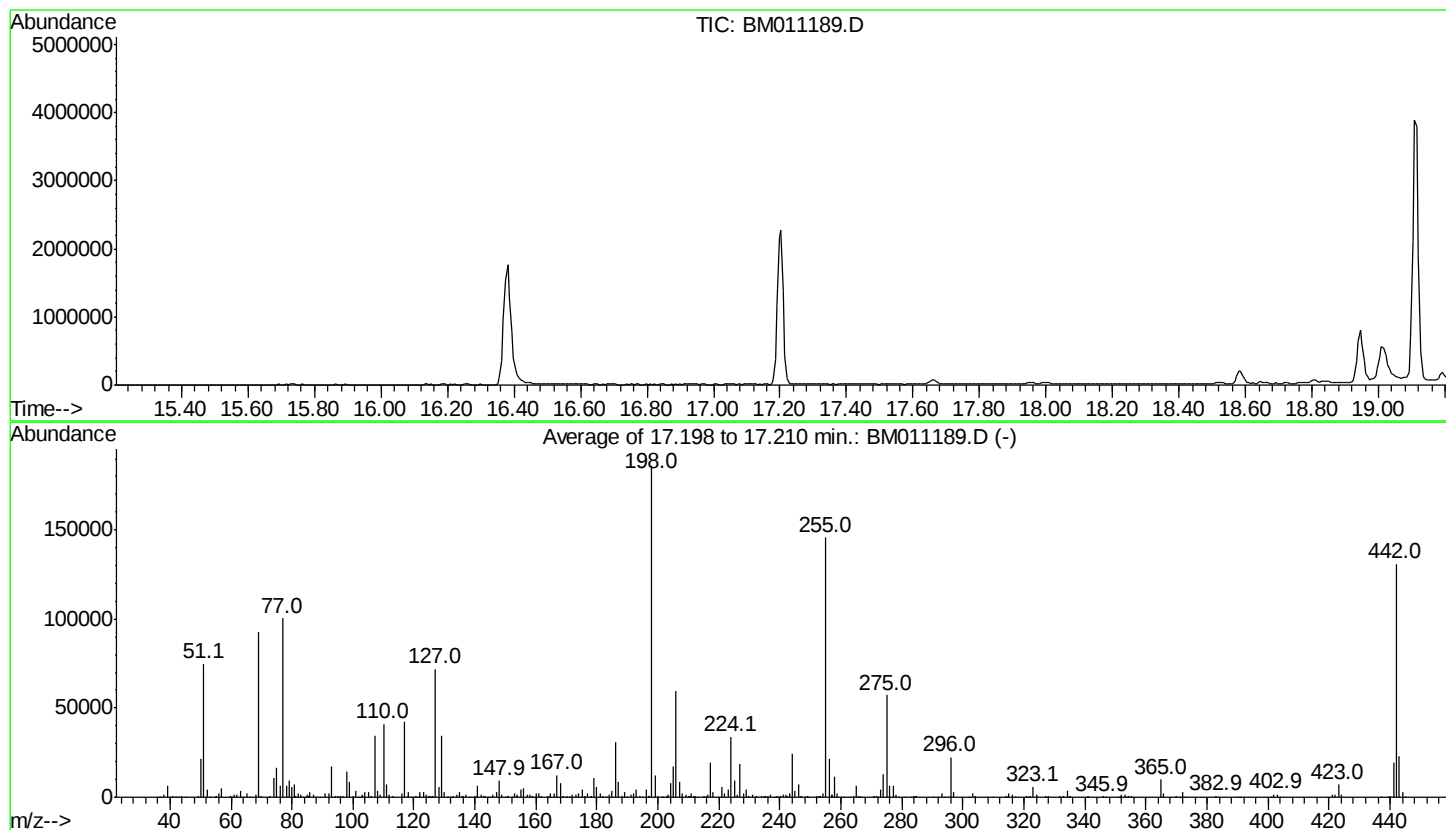

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	74773	PASS
68	69	0.00	2	1.2	1146	PASS
69	198	0.00	100	49.6	92342	PASS
70	69	0.00	2	0.7	650	PASS
127	198	10	80	38.7	72040	PASS
197	198	0.00	2	0.5	995	PASS
198	198	100	100	100.0	186069	PASS
199	198	5	9	6.7	12446	PASS
275	198	10	60	30.8	57346	PASS
365	198	1	100	5.3	9792	PASS
441	443	0.01	100	82.4	19234	PASS
442	198	50	100	70.4	130904	PASS
443	442	15	24	17.8	23338	PASS