
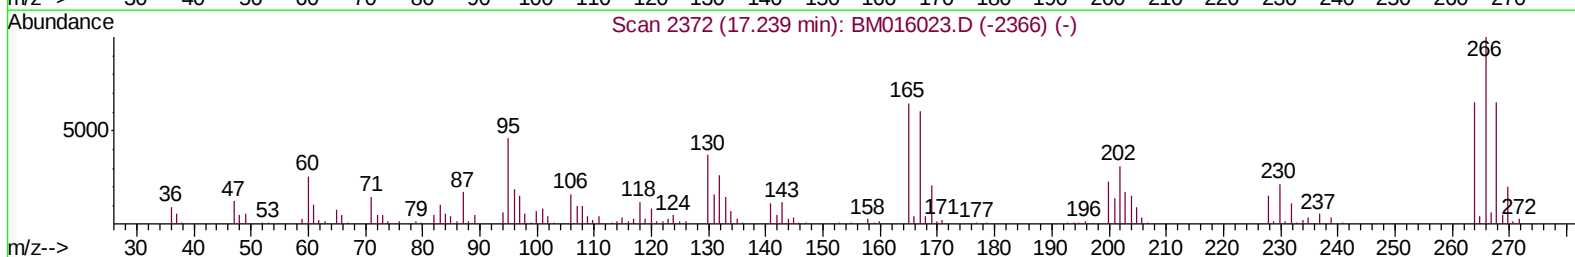
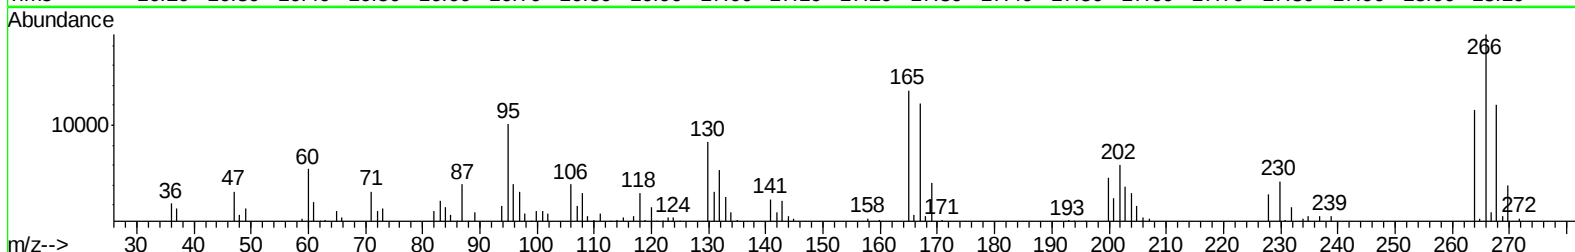


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080918\
Data File : BM016273.D
Acq On : 09 Aug 2018 09:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 07:45:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 16:23:37 2018
Response via : Initial Calibration

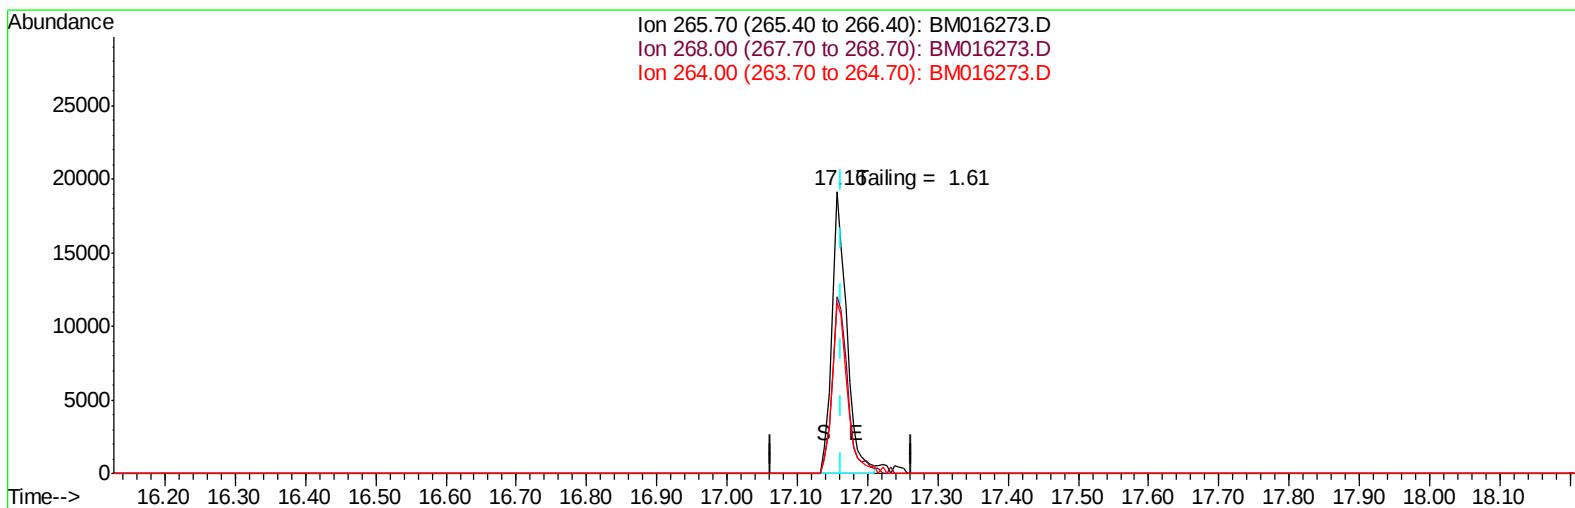

TIC: BM016273.D

(69) Pentachlorophenol (C)




17.157min (-0.006) 0.00ng

response 28109

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.75
264.00	61.20	60.36
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080918\
Data File : BM016273.D
Acq On : 09 Aug 2018 09:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 07:45:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 16:23:37 2018
Response via : Initial Calibration

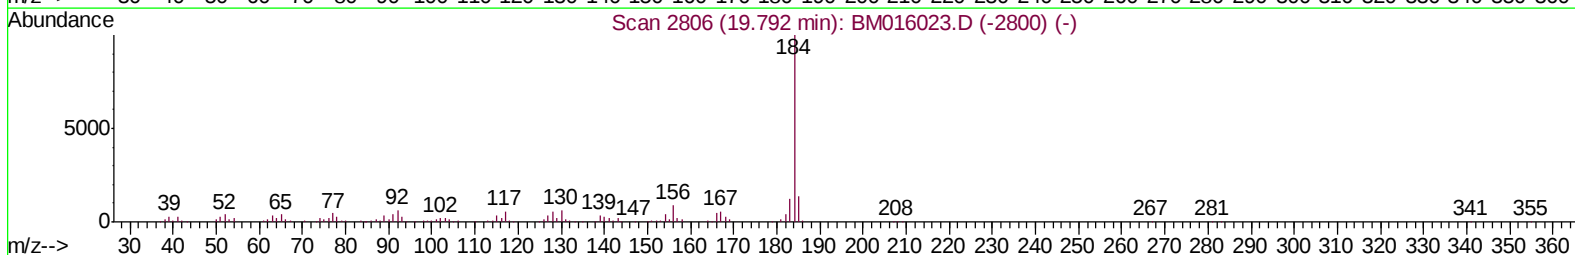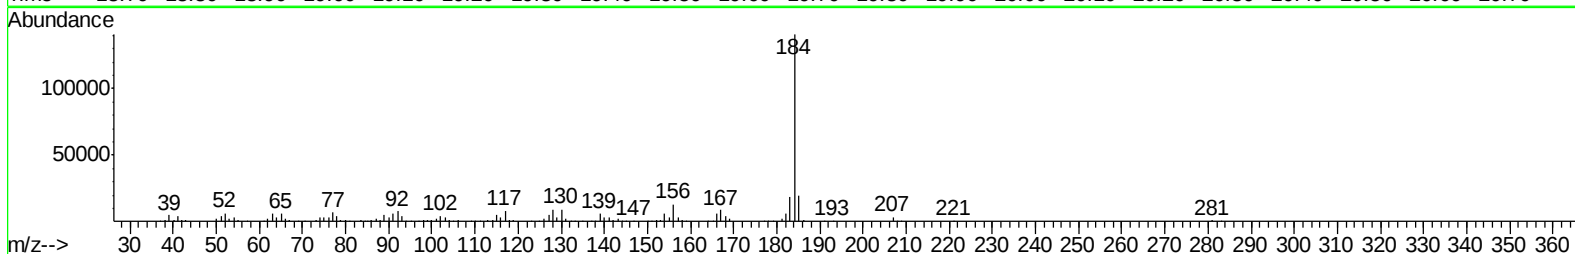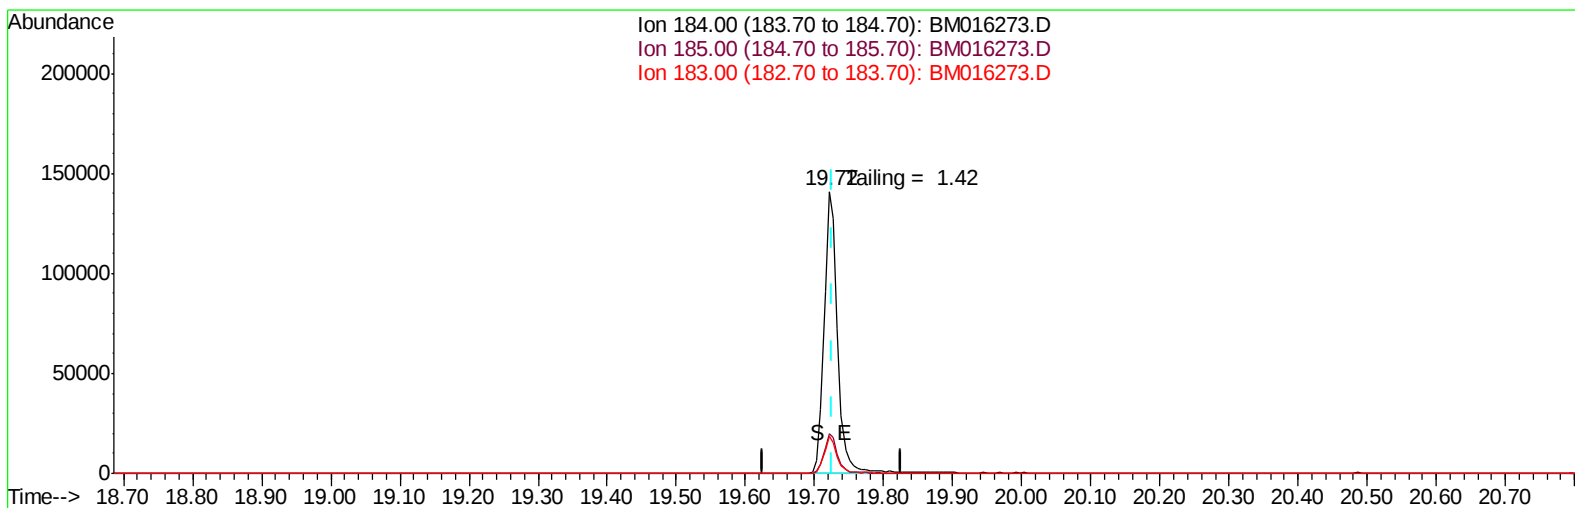

TIC: BM016273.D

(76) Benzidine

19.721min (-0.006) 15371.68ng

response 188573

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.95
183.00	11.10	13.07
0.00	0.00	0.00