
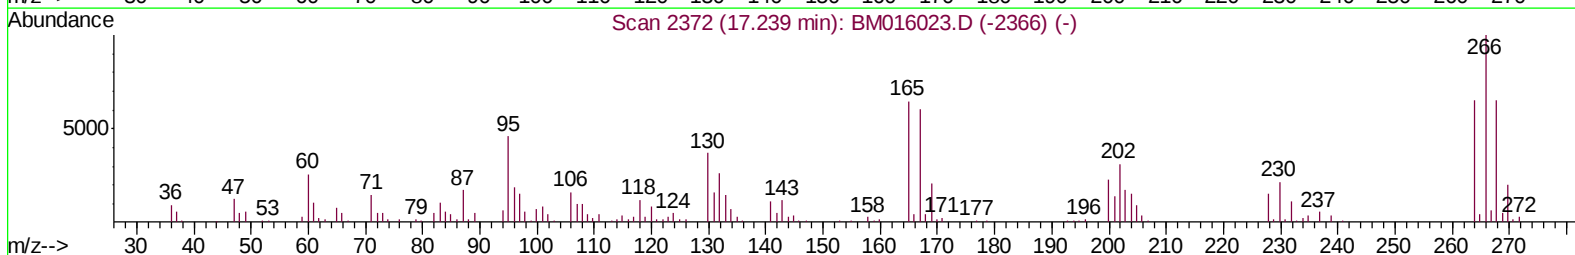
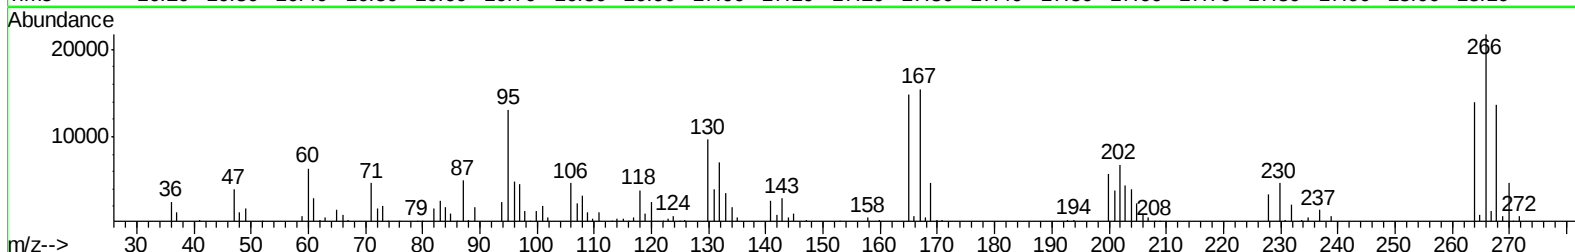


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080918\
Data File : BM016293.D
Acq On : 09 Aug 2018 22:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 07:33:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 16:23:37 2018
Response via : Initial Calibration

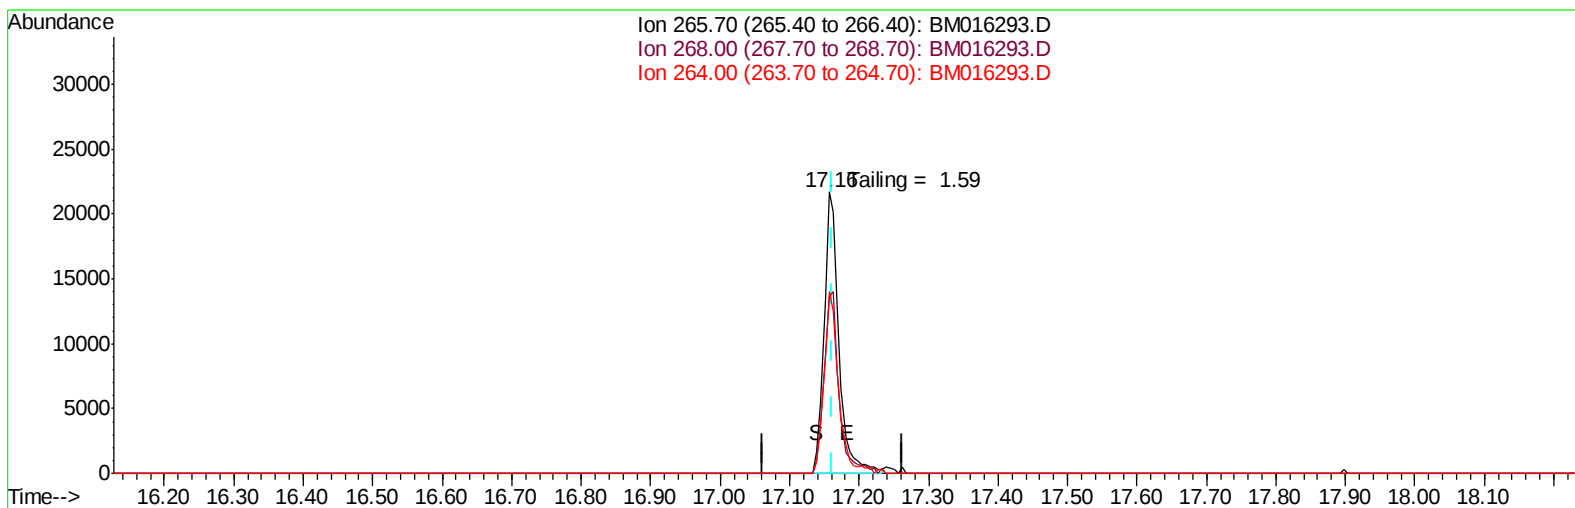

TIC: BM016293.D

(69) Pentachlorophenol (C)




17.157min (-0.006) 0.00ng

response 32328

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.62
264.00	61.20	64.36
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080918\
 Data File : BM016293.D
 Acq On : 09 Aug 2018 22:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 07:33:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 16:23:37 2018
 Response via : Initial Calibration

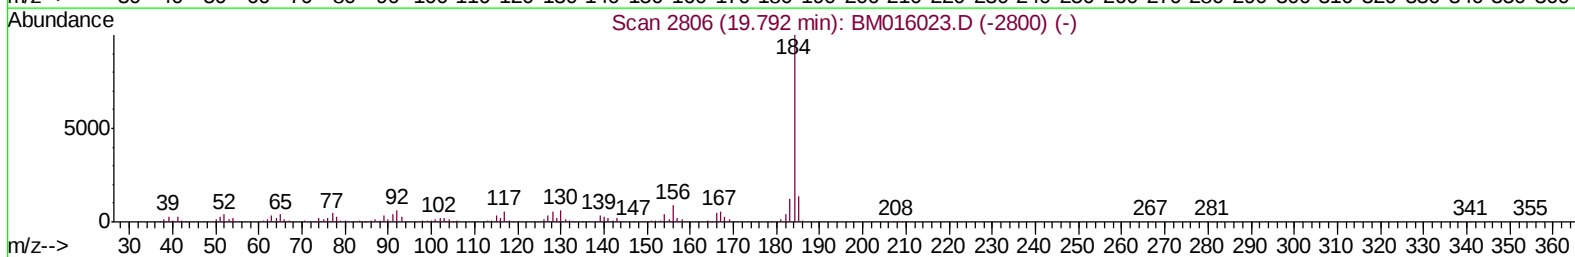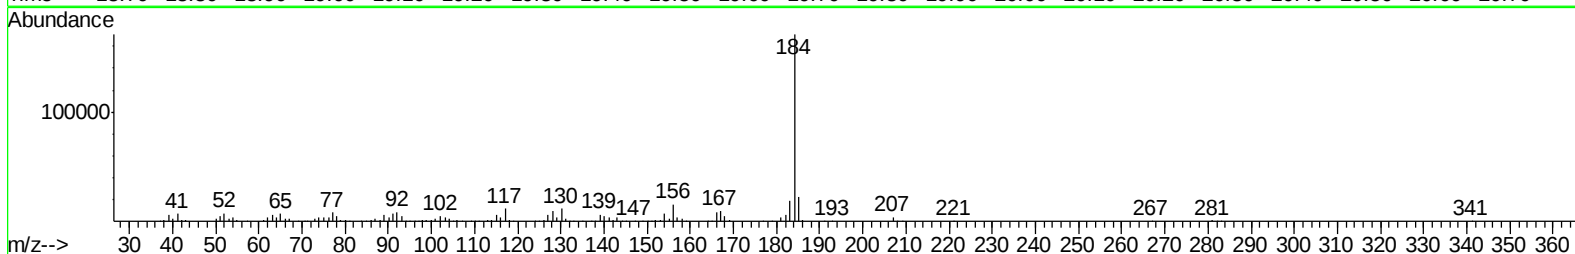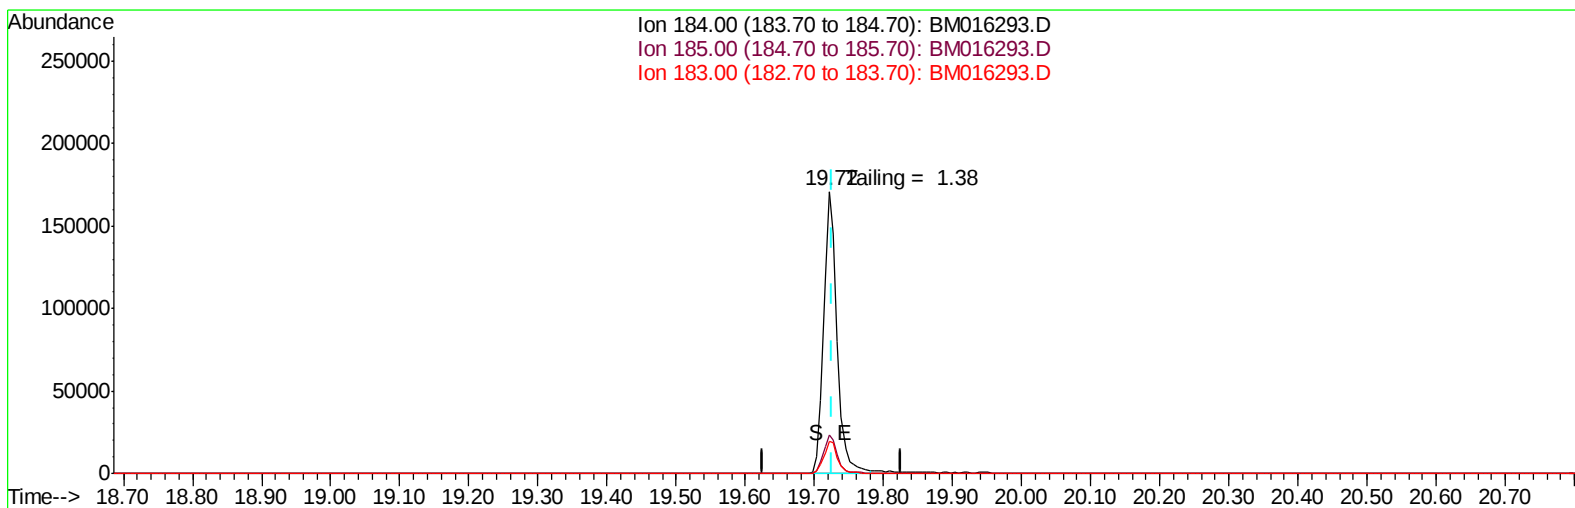

TIC: BM016293.D

(76) Benzidine

19.721min (-0.006) 24425.27ng

response 229336

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.47
183.00	11.10	11.46
0.00	0.00	0.00