


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080918\
 Data File : BM016273.D
 Acq On : 09 Aug 2018 09:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 16:23:37 2018

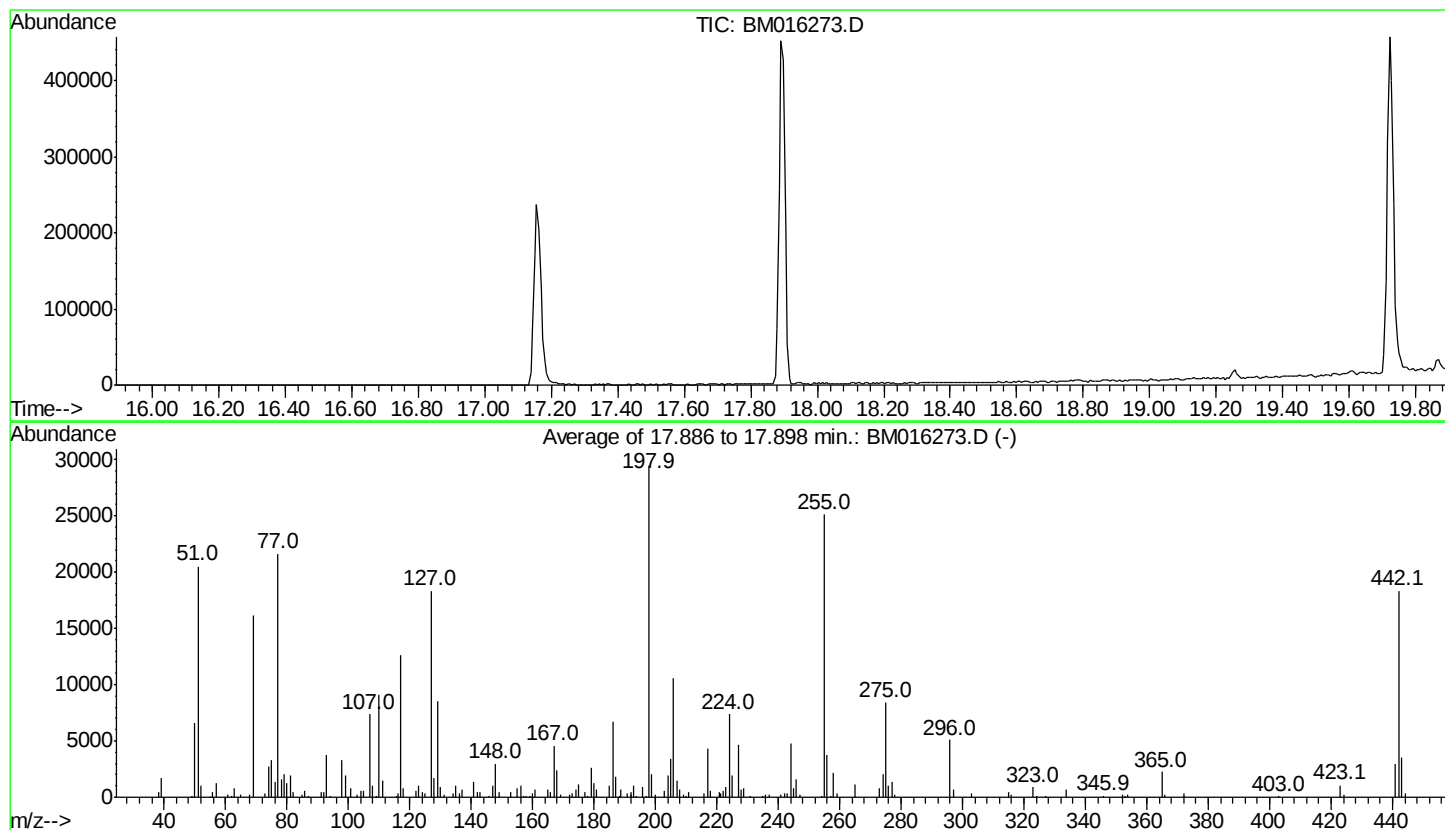

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.6	20509	PASS
68	69	0.00	2	1.6	259	PASS
69	198	0.00	100	54.7	16111	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	62.2	18306	PASS
197	198	0.00	2	0.5	133	PASS
198	198	100	100	100.0	29450	PASS
199	198	5	9	6.9	2026	PASS
275	198	10	60	28.5	8402	PASS
365	198	1	100	7.7	2267	PASS
441	198	0.01	100	9.9	2915	PASS
442	198	50	100	62.3	18347	PASS
443	442	15	24	19.1	3504	PASS