


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080918\
 Data File : BM016293.D
 Acq On : 09 Aug 2018 22:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 16:23:37 2018

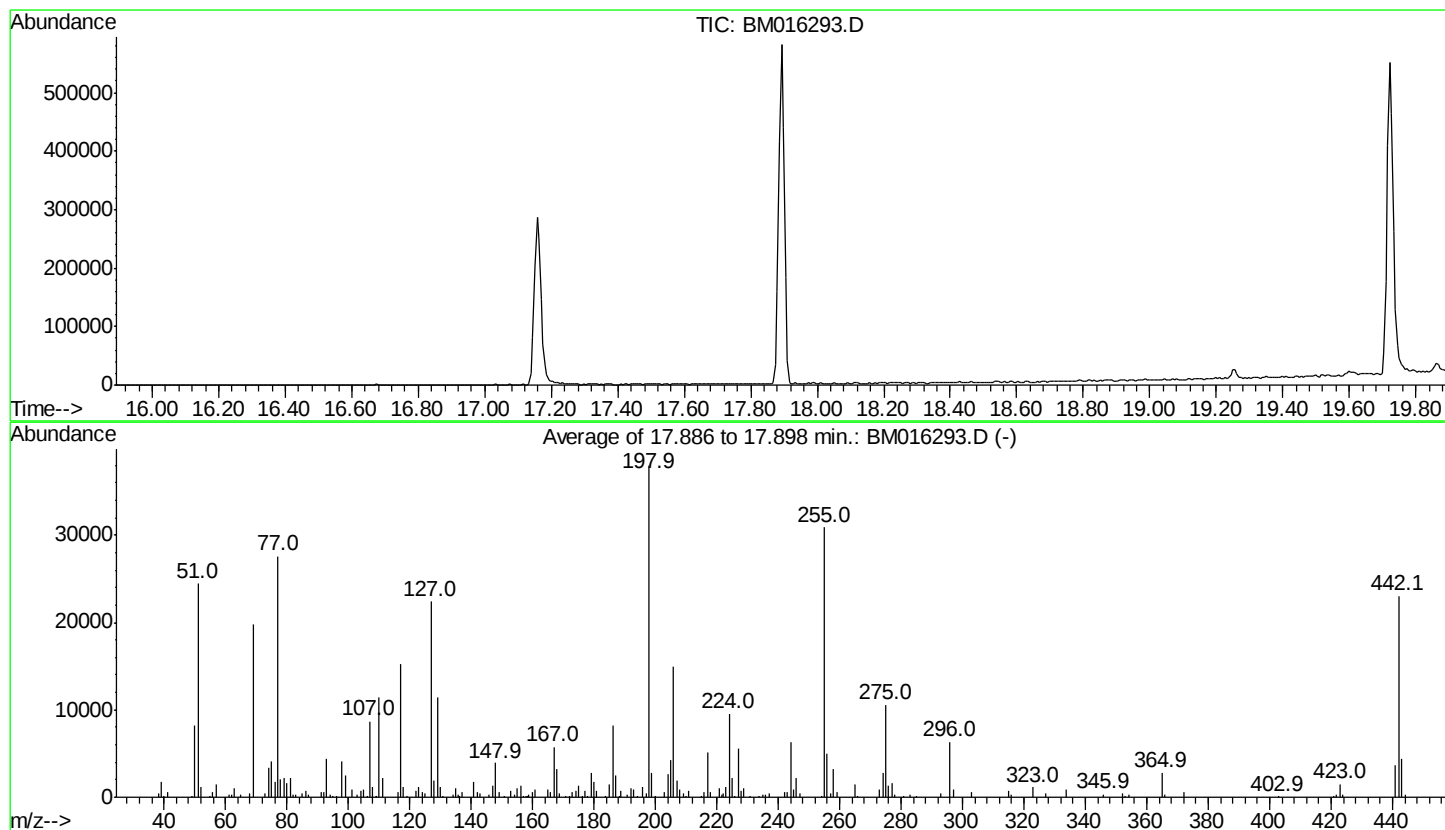

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.4	24424	PASS
68	69	0.00	2	2.1	407	PASS
69	198	0.00	100	52.0	19729	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.0	22376	PASS
197	198	0.00	2	1.1	401	PASS
198	198	100	100	100.0	37949	PASS
199	198	5	9	7.2	2744	PASS
275	198	10	60	28.0	10617	PASS
365	198	1	100	7.5	2849	PASS
441	198	0.01	100	9.8	3730	PASS
442	198	50	100	60.7	23024	PASS
443	442	15	24	19.1	4397	PASS