
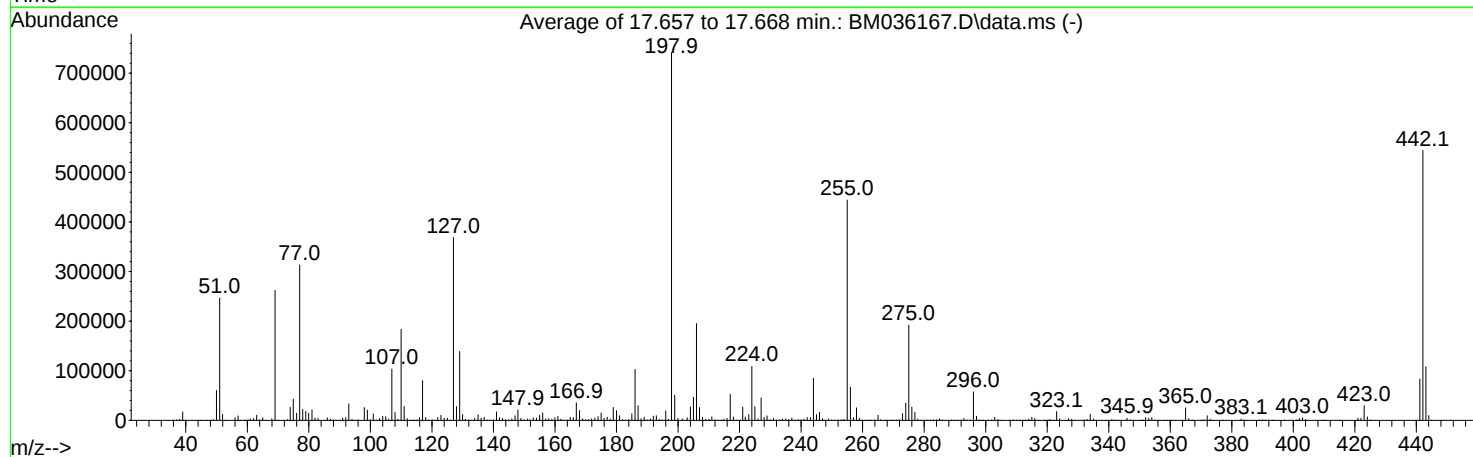


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080922\
 Data File : BM036167.D
 Acq On : 09 Aug 2022 09:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 10 22:19:26 2022

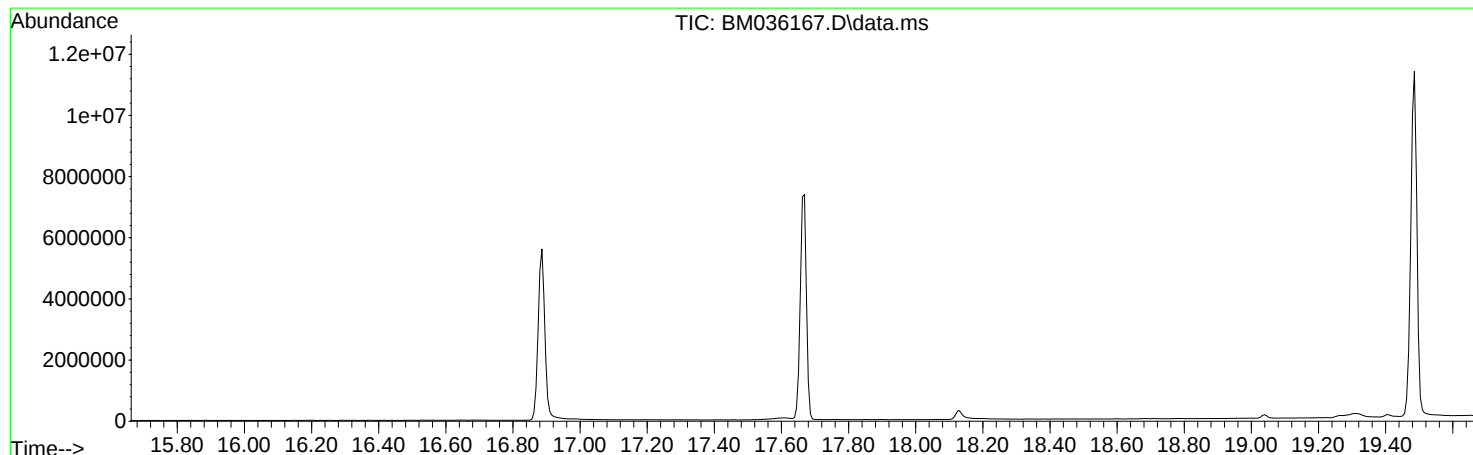




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	246642	PASS
68	69	0.00	2	1.3	3376	PASS
69	198	0.00	100	35.4	262276	PASS
70	69	0.00	2	0.1	329	PASS
127	198	10	80	49.7	368667	PASS
197	198	0.00	2	0.3	1926	PASS
198	198	100	100	100.0	741739	PASS
199	198	5	9	6.8	50723	PASS
275	198	10	60	25.9	192067	PASS
365	198	1	100	3.4	25067	PASS
441	198	0.01	100	11.3	83448	PASS
442	442	50	100	100.0	544171	PASS
443	442	15	24	19.8	108013	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080922\
Data File : BM036167.D
Acq On : 09 Aug 2022 09:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 10 08:51:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 23:36:56 2022
Response via : Initial Calibration

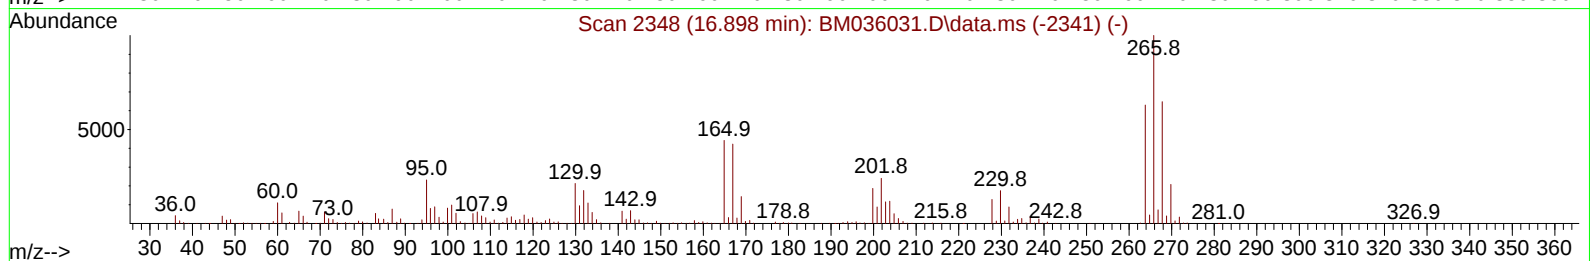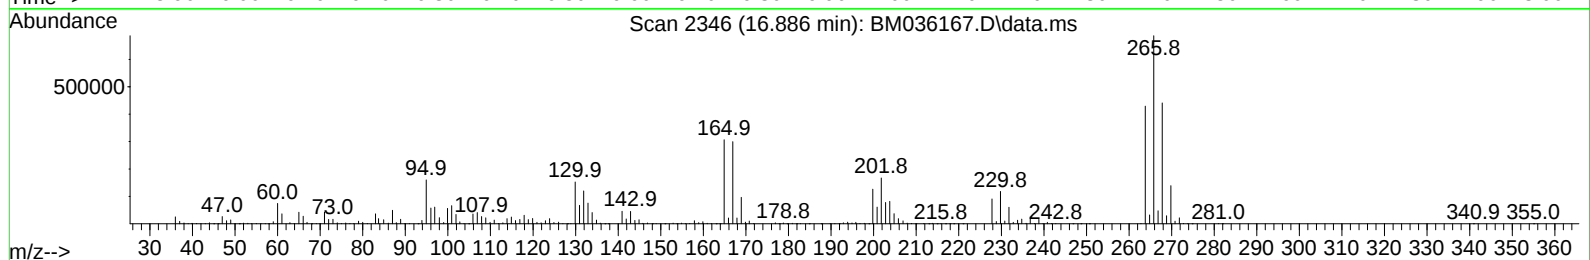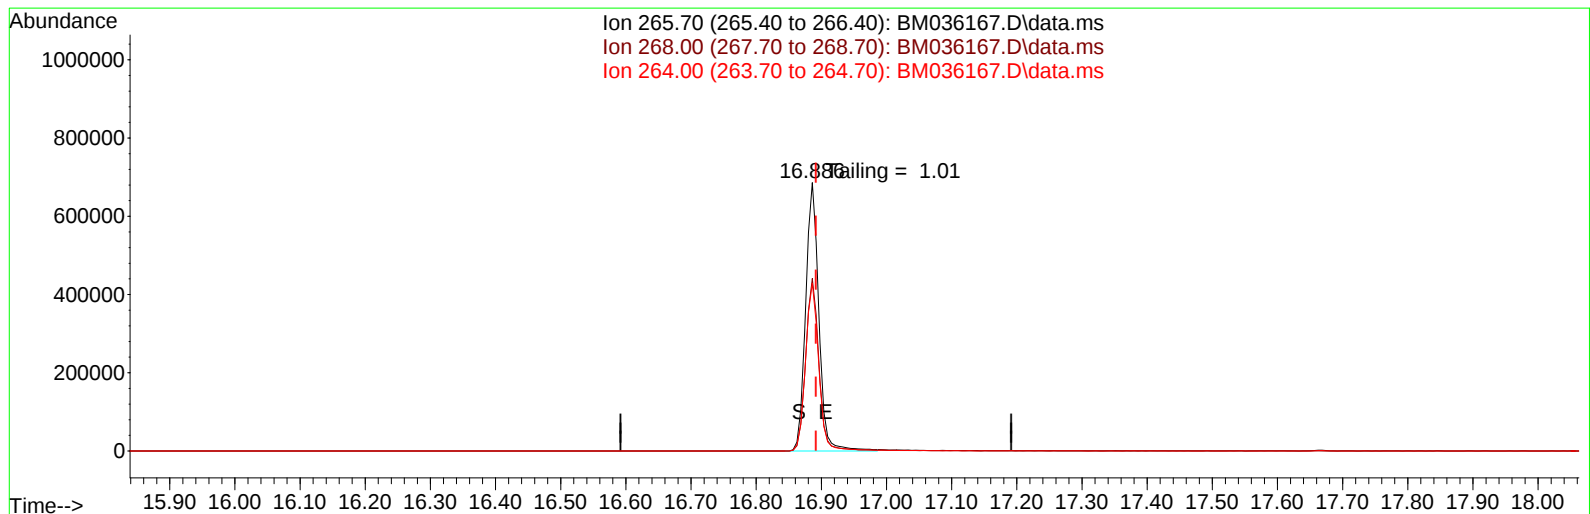

TIC: BM036167.D\data.ms

(70) Pentachlorophenol (C)

16.886min (-0.006) 460572.06 ng




response 975170

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.30
264.00	63.30	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080922\
 Data File : BM036167.D
 Acq On : 09 Aug 2022 09:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 10 08:51:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 23:36:56 2022
 Response via : Initial Calibration

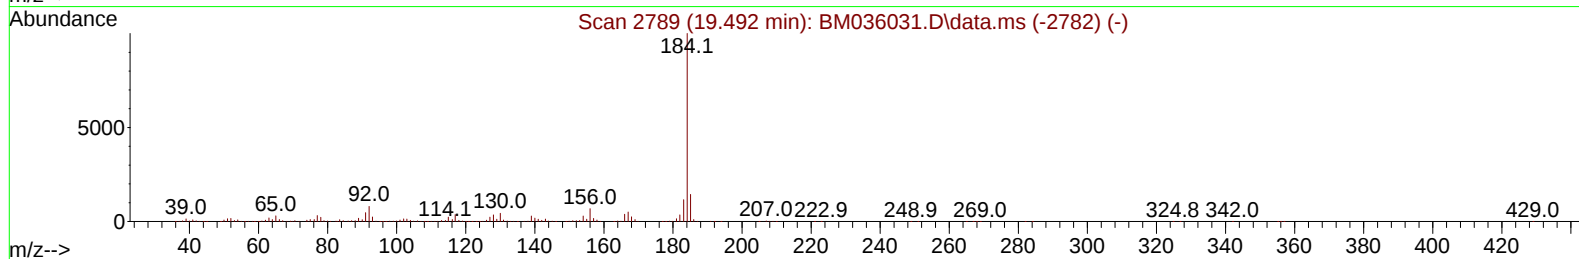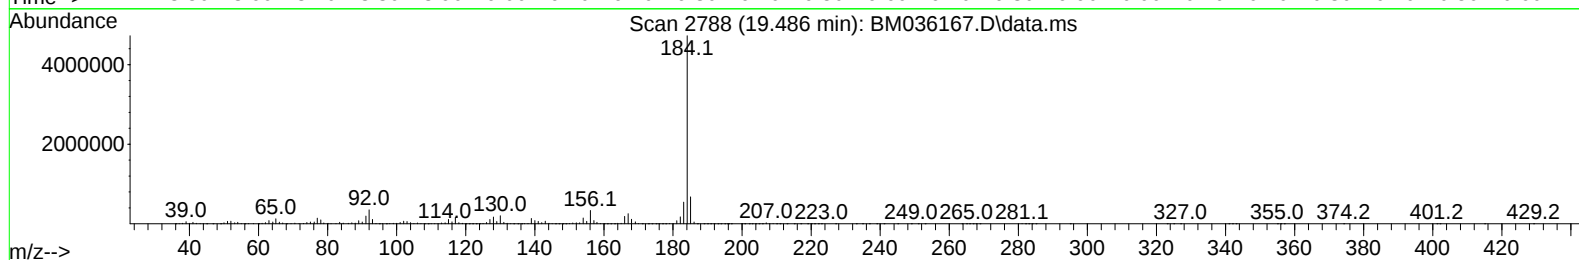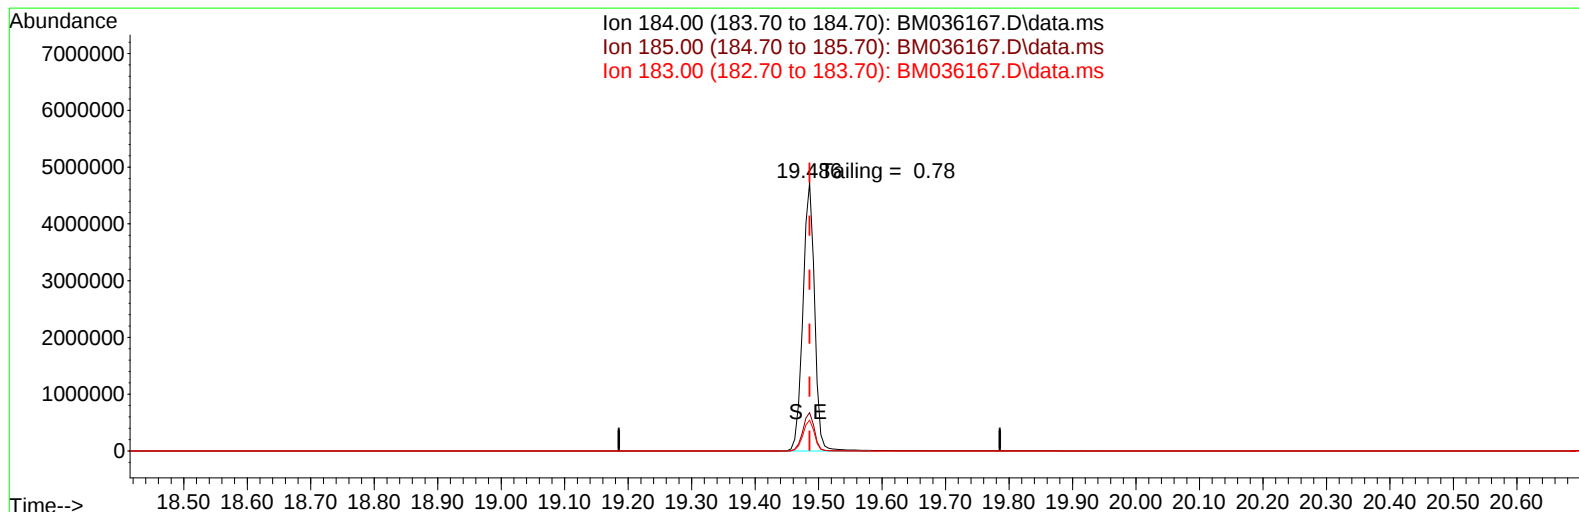

TIC: BM036167.D\data.ms

(77) Benzidine

19.486min (+ 0.000) 151641.17 ng

response 6099324

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.30
183.00	11.90	11.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/9/2022	BNA_M	<u>BM036167.D</u>
Compound Name	Response	Retention Time
DDT	2839089	20.703
DDD	38258	20.268
DDE	3576	19.756
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41834	2880923	1.45

Instrument :
BNA_M
ClientSampleId :
DFTPP